Draft for Public Comment

Form 36

DPC: 23/30446135 DC

BSI Group Headquarters

389 Chiswick High Road London W4 4AL

Tel: +44 (0)20 8996 9000
Fax: +44 (0)20 8996 7400
www.bsigroup.com

Date: 11 October 2023
Origin: European

Latest date for receipt of comments: 04 December 2023

Project No. 2021/02935

Responsible committee: CH/212 IVDs

Interested committees:

Title: Draft BS EN ISO 1135-5 Transfusion equipment for medical use. Part 5: Transfusion sets for single use with pressure infusion apparatus.
Please notify the secretary if you are aware of any keywords that might assist in classifying or identifying the standard or if the content of this standard i) has any issues related to 3rd party IPR, patent or copyright ii) affects other national standard(s) iii) requires additional national guidance or information

WARNING: THIS IS A DRAFT AND MUST NOT BE REGARDED OR USED AS A BRITISH STANDARD. THIS DRAFT IS NOT CURRENT BEYOND 04 December 2023

This draft is issued to allow comments from interested parties; all comments will be given consideration prior to publication. No acknowledgement will normally be sent. **See overleaf for information on the submission of comments.**

No copying is allowed, in any form, without prior written permission from BSI except as permitted under the Copyright, Designs and Patent Act 1988 or for circulation within a nominating organization for briefing purposes. Electronic circulation is limited to dissemination by e-mail within such an organization by committee members.

Further copies of this draft may be purchased from BSI Shop http://shop.bsigroup.com or from BSI Customer Services, Tel: +44(0) 20 8996 9001 or email cservices@bsigroup.com. British, International and foreign standards are also available from BSI Customer Services.

Information on the co-operating organizations represented on the committees referenced above may be obtained from https://standardsdevelopment.bsigroup.com/.

Responsible Committee Secretary: Ms Helena Barrell (BSI)
Direct tel:
E-mail: helena.barrell@bsigroup.com

Documents
Document Sharing Hub
Full document details: 23/30446135 DC

Introduction

This draft standard is based on national and international discussions. Your comments on this draft are invited and will assist in the preparation of the consequent standard.

For international standards, comments will be reviewed by the relevant UK national committee before sending the consensus UK vote and comments to the international committee, which will then decide appropriate action. If the international standard is approved, it is usual for the text to be published as a British Standard.

For national standards, comments will be reviewed by the relevant UK national committee and the resulting standards published as a British Standard.

UK Vote

Please indicate whether you consider the UK should submit a negative (with supporting technical reasons) or positive vote on this draft. Please indicate if you are aware of any reason why this draft standard should not be published as a British Standard.

Submission of Comments

- **Annotated drafts are not acceptable and will be rejected.**
- All comments should be submitted online at **https://standardsdevelopment.bsigroup.com/**. You will need to register in order to comment.

Template for comments and secretariat observations

Date: xx/xx/20xx	Document: ISO/DIS xxxx

1	2	(3)	4	5	(6)	7
MB	Clause No./ Subclause No./Annex **(e.g. 3.1)**	Paragraph/ Figure/Table/Note	**Type of comment**	**Commend (justification for change) by the MB**	**Proposed change by the MB**	**Secretariat observations on each comment submitted**
	3.1	Definition 1	ed	Definition is ambiguous and needs clarifying.	Amend to read '...so that the mains connector to which no connection...'	
	6.4	Paragraph 2	te	The use of the UV photometer as an alternative cannot be supported as serious problems have been encountered in its use in the UK.	Delete reference to UV photometer.	

Documents
Document Sharing Hub

Full document details: 23/30446135 DC

DRAFT INTERNATIONAL STANDARD

ISO/DIS 1135-5

ISO/TC **76**

Secretariat: **DIN**

Voting begins on:
2023-10-11

Voting terminates on:
2024-01-03

Transfusion equipment for medical use —

Part 5:
Transfusion sets for single use with pressure infusion apparatus

Matériel de transfusion à usage médical —

Partie 5: Appareils de transfusion non réutilisables avec les appareils de perfusion sous pression

ICS: 11.040.20

This document is circulated as received from the committee secretariat.

ISO/CEN PARALLEL PROCESSING

THIS DOCUMENT IS A DRAFT CIRCULATED FOR COMMENT AND APPROVAL. IT IS THEREFORE SUBJECT TO CHANGE AND MAY NOT BE REFERRED TO AS AN INTERNATIONAL STANDARD UNTIL PUBLISHED AS SUCH.

IN ADDITION TO THEIR EVALUATION AS BEING ACCEPTABLE FOR INDUSTRIAL, TECHNOLOGICAL, COMMERCIAL AND USER PURPOSES, DRAFT INTERNATIONAL STANDARDS MAY ON OCCASION HAVE TO BE CONSIDERED IN THE LIGHT OF THEIR POTENTIAL TO BECOME STANDARDS TO WHICH REFERENCE MAY BE MADE IN NATIONAL REGULATIONS.

RECIPIENTS OF THIS DRAFT ARE INVITED TO SUBMIT, WITH THEIR COMMENTS, NOTIFICATION OF ANY RELEVANT PATENT RIGHTS OF WHICH THEY ARE AWARE AND TO PROVIDE SUPPORTING DOCUMENTATION.

Reference number
ISO/DIS 1135-5:2023(E)

© ISO 2023

Full document details: 23/30446135 DC

COPYRIGHT PROTECTED DOCUMENT

© ISO 2023

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

© ISO 2023 – All rights reserved

Documents
Document Sharing Hub

Full document details: 23/30446135 DC

Contents

Page

Foreword ... **iv**

1 Scope ... **1**

2 Normative references ... **1**

3 Terms and definitions ... **2**

4 General requirements ... **3**

5 Materials ... **3**

6 Physical requirements ... **4**
6.1 Particulate contamination ... 4
6.2 Leakage ... 4
6.3 Tensile strength ... 4
6.4 Closure-piercing device ... 4
6.5 Tubing ... 5
6.6 Filter for blood and blood components ... 5
6.7 Drip chamber and drip tube ... 5
6.8 Flow regulator ... 5
6.9 Flow rate of blood and blood components ... 5
6.10 Injection site ... 6
6.11 Male conical fitting ... 6
6.12 Protective caps ... 6
6.13 Post-occlusion bolus volume ... 6

7 Chemical requirements ... **6**
7.1 Reducing (oxidizable) matter ... 6
7.2 Metal ions ... 6
7.3 Titration acidity or alkalinity ... 6
7.4 Residue on evaporation ... 7
7.5 UV absorption of extract solution ... 7

8 Biological requirements ... **7**
8.1 General ... 7
8.2 Sterility ... 7
8.3 Pyrogenicity ... 7
8.4 Haemolysis ... 7
8.5 Toxicity ... 7
8.6 Assessment of blood component depletion ... 7
8.7 Assessment of damage to blood components ... 8

9 Labelling ... **8**
9.1 General ... 8
9.2 Unit container ... 8
9.3 Shelf or multi-unit container ... 9

10 Packaging ... **9**

11 Disposal ... **9**

Annex A (normative) **Physical tests** ... **10**

Annex B (normative) **Chemical tests** ... **15**

Annex C (normative) **Biological tests** ... **17**

Annex D (normative) **Determination of tube volumes** ... **18**

Annex ZA (informative) **Relationship between this European standard and the General Safety and Performance Requirements of Regulation (EU) 2017/745 aimed to be covered** ... **20**

Documents
Document Sharing Hub

© ISO 2023 – All rights reserved

Full document details: 23/30446135 DC

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 76, *Transfusion, infusion and injection, and blood processing equipment for medical and pharmaceutical use,* in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/TC 205, *Non-active medical devices,* in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

This second edition of ISO 1135-5 cancels and replaces the first edition (ISO 1135-5:2015), which has been technically revised with the following changes:

— the definitions of the different ‘volume’ terms have been amended;

— 6.10 “Injection site” has been amended in regard of the use of needle-free injection ports and Luer-activated devices;

— 6.12 “Protective caps” has been more clarified how to prevent contamination;

— 6.13 has been completely revised and renamed to clarify the described volume;

— Clause 9 “Labelling” has been updated especially in regard of the referenced ISO 15223-1;

— Clause 10 “Packaging” has been amended by a reference to ISO 11607-1;

— Annex A “Physical test” has been amended by a general introduction on the pre-conditioning. In addition the description of the test for leakage has been extended;

— Annex D on ‘Storage volume’ has been renamed to ‘Determination of tube volumes’ and revised; D.3 on ‘Labelling’ has been deleted;

— the Normative references have been updated;

— some minor editorial changes were introduced in the whole document.

A list of all parts in the ISO 1135 series can be found on the ISO website.

© ISO 2023 – All rights reserved
Documents
Document Sharing Hub
Full document details: 23/30446135 DC

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

© ISO 2023 – All rights reserved

Documents
Document Sharing Hub
Full document details: 23/30446135 DC

Documents
Document Sharing Hub

Transfusion equipment for medical use —

Part 5: Transfusion sets for single use with pressure infusion apparatus

1 Scope

This document specifies requirements for single use transfusion sets for use with pressure infusion equipment capable of generating pressures up to 200 kPa (2 bar). This International Standard ensures compatibility with containers for blood and blood components as well as intravenous equipment.

Secondary aims of this document are to provide guidance on specifications relating to the quality and performance of materials used in transfusion sets, to present designations for transfusion set components, and to ensure the compatibility of sets with red cell and plasma blood components.

Platelet components should not be transfused under pressure using these sets.

NOTE In some countries, the national pharmacopoeia or other national regulations are legally binding and take precedence over this document.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 3826-1:2019, *Plastics collapsible containers for human blood and blood components — Part 1: Conventional containers*

ISO 3826-2, *Plastics collapsible containers for human blood and blood components — Part 2: Graphical symbols for use on labels and instruction leaflets*

ISO 10993-1, *Biological evaluation of medical devices — Part 1: Evaluation and testing within a risk management process*

ISO 10993-4, *Biological evaluation of medical devices — Part 4: Selection of tests for interactions with blood*

ISO 11607-1, *Packaging for terminally sterilized medical devices — Part 1: Requirements for materials, sterile barrier systems and packaging systems*

ISO 14644-1, *Cleanrooms and associated controlled environments — Part 1: Classification of air cleanliness by particle concentration*

ISO 15223-1, *Medical devices — Symbols to be used with information to be supplied by the manufacturer — Part 1: General requirements*

ISO 80369-7, *Small-bore connectors for liquids and gases in healthcare applications — Part 7: Connectors for intravascular or hypodermic applications*

ISO 80369-20, *Small-bore connectors for liquids and gases in healthcare applications — Part 20: Common test methods*

© ISO 2023 – All rights reserved

AVA Documents Document Sharing Hub
Full document details: 23/30446135 DC

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

— ISO Online browsing platform: available at https://www.iso.org/obp

— IEC Electropedia: available at https://www.electropedia.org/

3.1
filling volume
V_F
volume of tube during "pressureless" filling, respectively filling by gravity downstream of the infusion pump

Note 1 to entry: The tube remains unstressed.

Note 2 to entry: The filling volume is to be equated with the calculated volume of the tube.

3.2
storage volume
V_S
tube volume during pressurization downstream of the infusion pump

3.3
post-occlusion bolus volume
V_B
increased tube volume downstream of the infusion pump during pressurization in comparison with the unstressed tube

Note 1 to entry: V_B equals to $V_S - V_F$ considering that for V_S and V_F the tubes have the same length.

Note 2 to entry: For illustration of the post-occlusion bolus volume, see Figure 1.

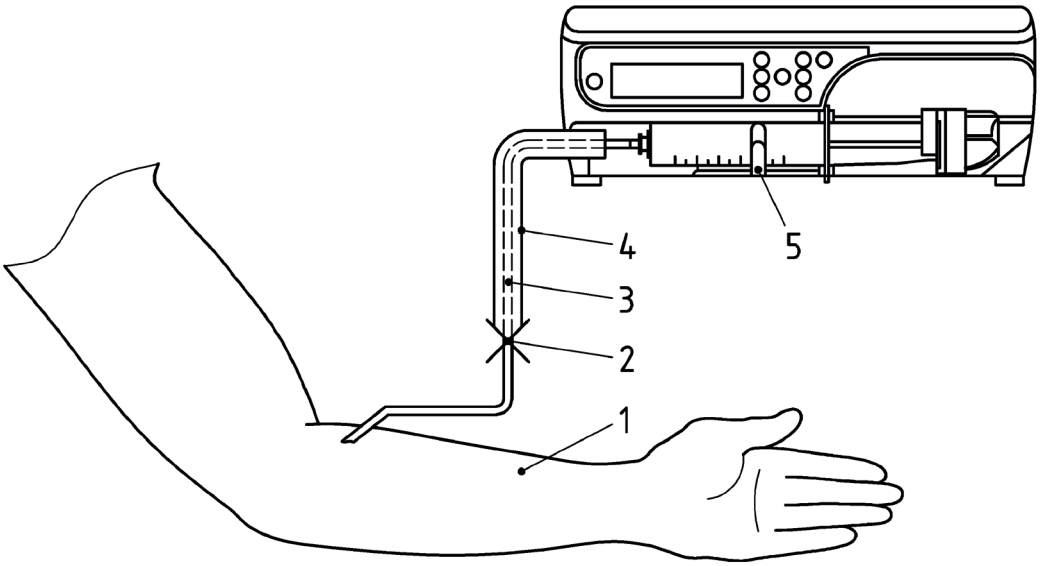

Key

1 patient
2 occlusion
3 tube
4 post-occlusion bolus volume
5 syringe pump

Figure 1 — Post-occlusion bolus volume

© ISO 2023 – All rights reserved
Documents
Document Sharing Hub
Full document details: 23/30446135 DC