



DPC: 24/30468668 DC

BSI Group Headquarters

389 Chiswick High Road London W4 4AL

Tel: +44 (0)20 8996 9000

Fax: +44 (0)20 8996 7400

www.bsigroup.com

Date: 03 June 2024

Origin: International

Latest date for receipt of comments: 27 July 2024

Project No. 2023/00164

Responsible committee: EH/3/8 Radioactivity measurements methods

Interested committees:

Title: Draft BS ISO 19383 BS ISO 13165-4 Water quality - Radium-226. Part 4: Test method using alpha spectrometry.

Please notify admin.start@bsigroup.com if you are aware of any keywords that might assist in clarifying or identifying the standard or of the content of this standard:

- i) has any issues related to 3rd party IPR, patent or copyright
- ii) affects other national standard(s)
- iii) requires additional national guidance or information

WARNING: THIS IS A DRAFT AND MUST NOT BE REGARDED OR USED AS A BRITISH STANDARD. THIS DRAFT IS NOT CURRENT BEYOND 27 July 2024

This draft is issued to allow comments from interested parties; all comments will be given consideration prior to publication. No acknowledgement will normally be sent. **See overleaf for information on the submission of comments.**

No copying is allowed, in any form, without prior written permission from BSI except as permitted under the Copyright, Designs and Patent Act 1988 or for circulation within a nominating organization for briefing purposes. Electronic circulation is limited to dissemination by e-mail within such an organization by committee members.

Further copies of this draft may be purchased from BSI Shop <http://shop.bsigroup.com> or from BSI Customer Services, Tel: +44(0) 20 8996 9001 or email cservices@bsigroup.com. British, International and foreign standards are also available from BSI Customer Services.

Information on the co-operating organizations represented on the committees referenced above may be obtained from <https://standardsdevelopment.bsigroup.com/>.

E-mail: admin.start@bsigroup.com

Introduction

This draft standard is based on national and international discussions. Your comments on this draft are invited and will assist in the preparation of the consequent standard.

For international standards, comments will be reviewed by the relevant UK national committee before sending the consensus UK vote and comments to the international committee, which will then decide appropriate action. If the international standard is approved, it is usual for the text to be published as a British Standard.

For national standards, comments will be reviewed by the relevant UK national committee and the resulting standards published as a British Standard.

UK Vote

Please indicate whether you consider the UK should submit a negative (with supporting technical reasons) or positive vote on this draft. Please indicate if you are aware of any reason why this draft standard should not be published as a British Standard.

Submission of Comments

- **Annotated drafts are not acceptable and will be rejected.**
- All comments should be submitted online at <https://standardsdevelopment.bsigroup.com/>. You will need to register in order to comment.

Template for comments and secretariat observations

Date: xx/xx/20xx	Document: ISO/DIS xxxx
------------------	------------------------

1	2	(3)	4	5	(6)	7
MB	Clause No./ Subclause No./Annex (e.g. 3.1)	Paragraph/ Figure/Table/Note	Type of comment	Comment (justification for change) by the MB	Proposed change by the MB	Secretariat observations on each comment submitted
	3.1	Definition 1	ed	Definition is ambiguous and needs clarifying.	Amend to read '...so that the mains connector to which no connection...'	
	6.4	Paragraph 2	te	The use of the UV photometer as an alternative cannot be supported as serious problems have been encountered in its use in the UK.	Delete reference to UV photometer.	



DRAFT International Standard

ISO/DIS 13165-4

Water quality — Radium-226 — Part 4: Test method using alpha spectrometry

ICS: 17.240; 13.060.60; 13.280

ISO/TC 147/SC 3

Secretariat: **AFNOR**

Voting begins on:
2024-06-03

Voting terminates on:
2024-08-26

This document is circulated as received from the committee secretariat.

THIS DOCUMENT IS A DRAFT CIRCULATED FOR COMMENTS AND APPROVAL. IT IS THEREFORE SUBJECT TO CHANGE AND MAY NOT BE REFERRED TO AS AN INTERNATIONAL STANDARD UNTIL PUBLISHED AS SUCH.

IN ADDITION TO THEIR EVALUATION AS BEING ACCEPTABLE FOR INDUSTRIAL, TECHNOLOGICAL, COMMERCIAL AND USER PURPOSES, DRAFT INTERNATIONAL STANDARDS MAY ON OCCASION HAVE TO BE CONSIDERED IN THE LIGHT OF THEIR POTENTIAL TO BECOME STANDARDS TO WHICH REFERENCE MAY BE MADE IN NATIONAL REGULATIONS.

RECIPIENTS OF THIS DRAFT ARE INVITED TO SUBMIT, WITH THEIR COMMENTS, NOTIFICATION OF ANY RELEVANT PATENT RIGHTS OF WHICH THEY ARE AWARE AND TO PROVIDE SUPPORTING DOCUMENTATION.

Reference number
ISO/DIS 13165-4:2024(en)

Full document details: 24/30468668 DC

© ISO 2024  **Documents**
Document Sharing Hub



COPYRIGHT PROTECTED DOCUMENT

© ISO 2024

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	2
4 Symbols	2
5 Principle	3
6 Sampling, handling, and storage	5
7 Procedure	6
8 Quality assurance and quality control program	6
8.1 General	6
8.2 Instrument verification	6
8.3 Contamination	6
8.4 Interference control	6
8.5 Alpha resolution	6
8.6 Method verification	7
8.7 Demonstration of analyst capability	7
9 Expression of results	7
9.1 General	7
9.2 Tracer activity added	7
9.3 Count rate and net count rate	7
9.4 Total recovery	8
9.5 Activity concentration of ^{226}Ra	8
9.6 Combined uncertainties	9
9.7 Decision threshold	9
9.8 Detection limit	10
9.9 Probabilistically symmetric coverage interval	10
9.9.1 Limits of the probabilistically symmetric coverage interval	10
9.9.2 The shortest coverage interval	10
10 Test report	11
Annex A (informative) Radioactive interferences and an example of alpha spectrum	13
Annex B (informative) Preparation of thin alpha source by electrodeposition	14
Annex C (informative) Preparation of thin alpha source by barium sulfate micro-precipitation	17
Annex D (informative) Method 1 — Radium separation using a solid phase extraction disc	19
Annex E (informative) Method 2 — Radium pre-concentration and separation with a MnO_2 resin followed by the removal of potential radioactive interferences using an extraction chromatography resin	21
Annex F (informative) Method 3 — Preconcentration of radium using CaCO_3 and then separation of Ra from potential interferences using a cation exchange resin followed by an extraction chromatography resin	24
Annex G (informative) Method 4 — Preconcentration of Ra using a lead sulfate coprecipitation and then separation of Ra from potential interferences using a masking agent	27
Bibliography	29

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

ISO draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at www.iso.org/patents. ISO shall not be held responsible for identifying any or all such patent rights.

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee *[or Project Committee]* ISO/TC 147 *Water quality*, Subcommittee SC 3, *Radioactivity measurements*.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

Radionuclides are present throughout the environment; thus, water bodies (e.g. surface waters, ground waters, sea waters) contain radionuclides, which can be of either natural or anthropogenic origin:

- naturally-occurring radionuclides, including ^3H , ^{14}C , ^{40}K and those originating from the thorium and uranium decay series, in particular ^{210}Pb , ^{210}Po , ^{222}Rn , ^{226}Ra , ^{228}Ra , ^{227}Ac , ^{232}Th , ^{231}Pa , ^{234}U , and ^{238}U , can be found in water bodies due to either natural processes (e.g., desorption from the soil and runoff by rain water) or released from technological processes involving naturally occurring radioactive materials (e.g. mining, mineral processing, oil, gas, and coal production, water treatment and the production and use of phosphate fertilisers);
- anthropogenic radionuclides such as ^{55}Fe , ^{59}Ni , ^{63}Ni , ^{90}Sr , ^{99}Tc , transuranic elements (e.g., Np, Pu, Am, and Cm), and some gamma emitting radionuclides such as ^{60}Co and ^{137}Cs can also be found in natural waters. Small quantities of anthropogenic radionuclides can be discharged from nuclear facilities to the environment as a result of authorized routine releases. The radionuclides present in liquid effluents are usually controlled before being discharged to the environment^[1] and water bodies. Anthropogenic radionuclides used for medical and industrial applications can be released to the environment after use. Anthropogenic radionuclides are also found in waters due to contamination from fallout resulting from above-ground nuclear detonations and accidents such as those that have occurred at the Chornobyl and Fukushima nuclear facilities.

Radionuclide activity concentrations in water bodies can vary according to local geological characteristics and climatic conditions and can be locally and temporally enhanced by releases from nuclear facilities during planned, existing, and emergency exposure situations.^{[2][3]} Some drinking water sources can thus contain radionuclides at activity concentrations that could present a human health risk. The World Health Organization (WHO) recommends to routinely monitor radioactivity in drinking waters^[4] and to take proper actions when needed to minimize the health risk.

National regulations usually specify the activity concentration limits that are authorized in drinking waters, water bodies, and liquid effluents to be discharged to the environment. These limits can vary for planned, existing, and emergency exposure situations. As an example, during either a planned or existing situation, the WHO guidance level for ^{226}Ra in drinking water is $1 \text{ Bq}\cdot\text{l}^{-1}$ ^[4], see NOTES 1 and 2. Compliance with these limits is assessed by measuring radioactivity in water samples and by comparing the results obtained, with their associated uncertainties, as specified by ISO/IEC Guide 98-3^[5] and ISO 5667-20^[6].

NOTE 1 If the value is not specified in Annex 6 of Reference [4], the value has been calculated using the formula provided in Reference [4] and the dose coefficient data from References [7] and [8].

NOTE 2 The guidance level calculated in Reference [4] is the activity concentration that results in an effective dose of $0,1 \text{ mSv}\cdot\text{a}^{-1}$ to members of the public for an intake of $2 \text{ l}\cdot\text{d}^{-1}$ of drinking water for one year. This is an effective dose that represents a very low level of risk to human health and which is not expected to give rise to any detectable adverse health effects^[4].

This document contains method(s) to support laboratories, which need to determine ^{226}Ra in water samples. The method(s) described in this document can be used for various types of waters (see [Clause 1](#)). Minor modifications such as sample volume and counting time can be made if needed to ensure that the decision threshold, detection limit, and uncertainties are below the required limits. This can be done for several reasons such as emergency situations, lower national guidance limits, and operational requirements.

Water quality — Radium-226 —

Part 4:

Test method using alpha spectrometry

WARNING — Persons using this document should be familiar with normal laboratory practice. This document does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user to establish appropriate safety and health practices and to determine the applicability of any other restrictions.

IMPORTANT — It is essential that tests conducted according to this document be carried out by suitably trained staff.

1 Scope

This document specifies methods to determine ^{226}Ra in all types of waters by alpha spectrometry.

The methods are applicable to test samples of supply/drinking water, rainwater, surface and ground water, marine water, as well as cooling water, industrial water, domestic, and industrial wastewater after proper sampling and handling, and test sample preparation.

The detection limit depends on the sample volume, the instrument used, the background count rate, the detection efficiency, the counting time, and the chemical yield. The detection limit of the methods described in this document, using currently available alpha spectrometry apparatus, is $\leq 3 \text{ mBq}\cdot\text{l}^{-1}$ (or $\text{mBq}\cdot\text{kg}^{-1}$), which is lower than the WHO criteria for safe consumption of drinking water ($1 \text{ Bq}\cdot\text{l}^{-1}$).^[4] This value can typically be achieved with a counting time of 48 h for a test sample volume of 40 ml.

The method described in this document is applicable in the event of an emergency situation. For an emergency situation, it is preferable to reduce the counting time rather than the sample volume.

Filtration of the test sample is necessary. The analysis of ^{226}Ra adsorbed to suspended matter is not covered by this method. The analysis of the insoluble fraction requires a mineralization step that is not covered by this document. In this case, the measurement is made on the different phases obtained. The final activity is the sum of all the measured activity concentrations.

It is the user's responsibility to ensure the validity of this test method for the water samples tested.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO/IEC Guide 99, *International vocabulary of metrology — Basic and general concepts and associated terms (VIM)*

ISO 5667-1, *Water quality — Sampling — Part 1: Guidance on the design of sampling programmes and sampling techniques*

ISO 5667-3, *Water quality — Sampling — Part 3: Preservation and handling of water samples*

ISO 5667-10, *Water quality — Sampling — Part 10: Guidance on sampling of waste water*

ISO 11929 (series), *Determination of the characteristic limits (decision threshold, detection limit and limits of the confidence interval) for measurements of ionizing radiation — Fundamentals and application*

ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories*

ISO 80000-10, *Quantities and units — Part 10: Atomic and nuclear physics*

3 Terms and definitions

No terms and definitions are listed in this document.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

4 Symbols

For the purposes of this document, the symbols and designations given in ISO 80000-10, ISO 11929 series, ISO/IEC Guide 98 3, and ISO/IEC Guide 99 and the following apply.

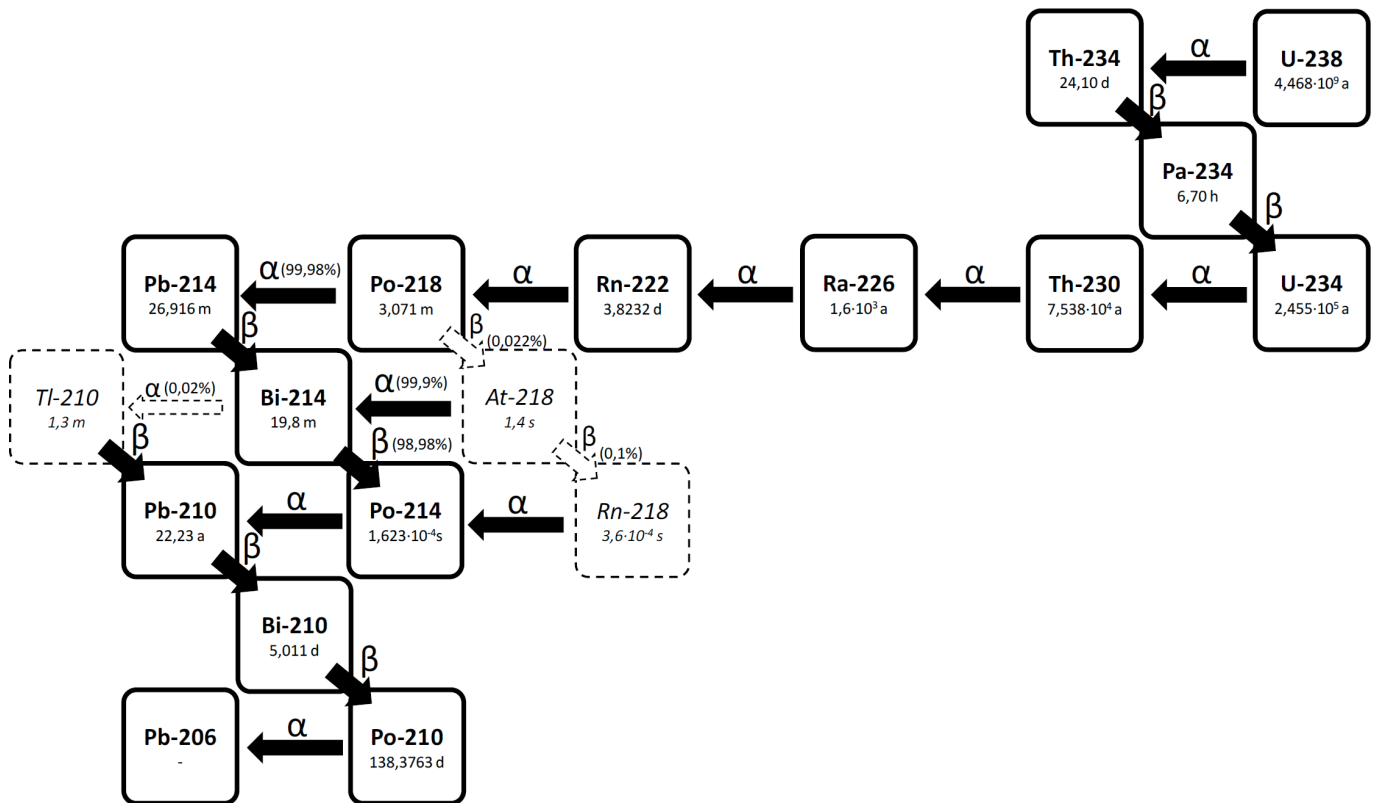
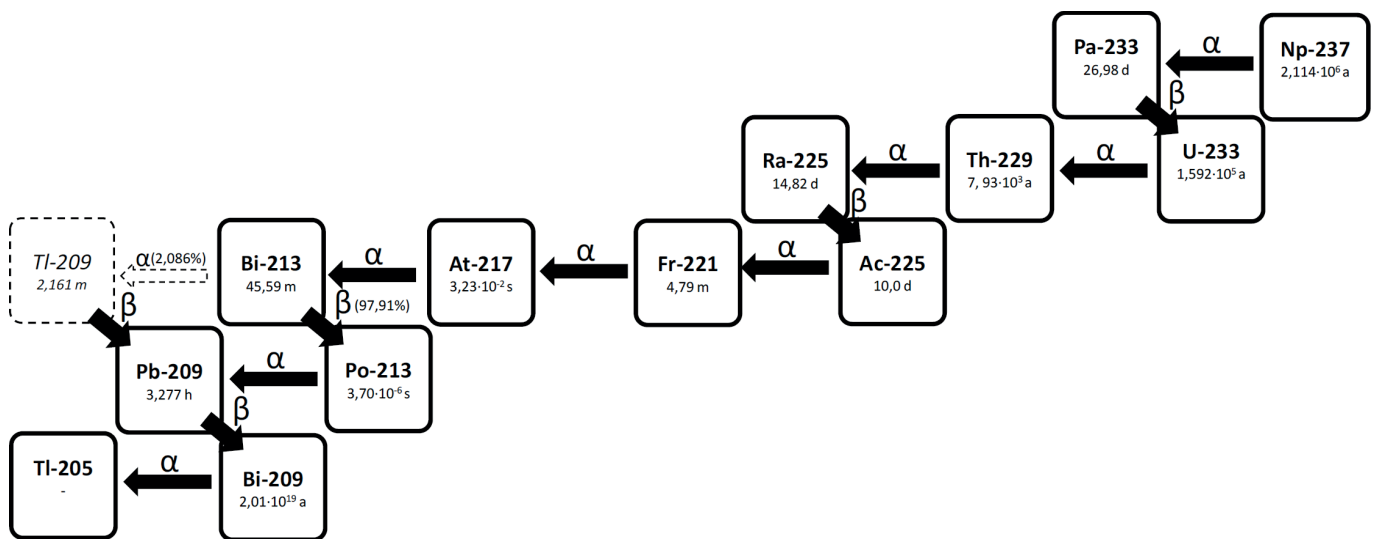
A_T	Activity of the ^{225}Ra tracer added	Bq
α	Probability of the false positive decision	
β	Probability of the false negative decision	
c_A	Activity concentration of ^{226}Ra measured in the sample	$\text{Bq}\cdot\text{l}^{-1}$
c_A^*	Decision threshold of the measurand	$\text{Bq}\cdot\text{l}^{-1}$
$c_A^\#$	Detection limit of the measurand	$\text{Bq}\cdot\text{l}^{-1}$
$c_A^{\triangleleft}, c_A^{\triangleleft}$	Lower and upper limits of the probabilistically symmetric coverage interval of the measurand, respectively	$\text{Bq}\cdot\text{l}^{-1}$
$c_A^{\leq}, c_A^{\geq}$	Lower and upper limits of the shortest coverage interval of the measurand, respectively	$\text{Bq}\cdot\text{l}^{-1}$
$\widetilde{c}_A$	Possible or assumed true quantity values of the measurand	$\text{Bq}\cdot\text{l}^{-1}$
c_{A_T}	Activity concentration of ^{225}Ra tracer solution at the moment of separation	$\text{Bq}\cdot\text{l}^{-1}$
ε	Counting efficiency	
Φ	Distribution function of the standardized normal distribution; $\Phi(k_p) = p$ applies	
$1-\gamma$	Probability for the coverage interval of the measurand	
k_p	Quantiles of the standardized normal distribution for the probabilities p (for instance $p = 1-\alpha$, $1-\beta$ or $1-\gamma/2$)	
k_q	Quantiles of the standardized normal distribution for the probabilities q (for instance $q = 1-\alpha$, $1-\beta$ or $1-\gamma/2$)	
λ	Decay constant of the isotope (ex: $\lambda_{^{215}\text{Po}}$ is the decay constant of ^{215}Po)	s^{-1}
m	Sample mass	kg
m_{ST}	Mass of tracer solution	g
N_0	Number of background counts measured on the alpha spectrum for a given time in the region of interest of ^{226}Ra , the measurand.	
N_{0T}	Number of background counts measured on the alpha spectrum for a given time in the region of interest of ^{217}At (progeny of ^{225}Ra tracer).	
N_g	Number of counts measured on the alpha spectrum for a given time in the region of interest of ^{226}Ra , the measurand.	
N_T	Number of counts measured on the alpha spectrum for a given time in the region of interest of ^{217}At (progeny of ^{225}Ra tracer).	
p	Probability for the coverage interval of the measurand	

q	Probability for the coverage interval of the measurand	
r_o	Background count rate in the region of interest of the measurand (^{226}Ra)	s^{-1}
r_{oT}	Background count rate in the tracer region of interest of the tracer (^{217}At) (progeny of ^{225}Ra tracer)	s^{-1}
R	Total recovery	
R_c	Chemical recovery	
r_g	Gross count rate in the region of interest of the measurand (^{226}Ra)	s^{-1}
r_{net}	Net count rate of the measurand (^{226}Ra)	s^{-1}
$r_{\text{net}T}$	Net count rate of the tracer progeny (^{217}At)	s^{-1}
$r_{\text{Anet}T}$	Apparent net count rate of the tracer (^{225}Ra)	s^{-1}
r_T	Gross count rate in the region of interest of the tracer progeny (^{217}At) (progeny of ^{225}Ra tracer)	s^{-1}
t	Time	s
$T_{1/2}$	Radioactive half-life of the isotope (ex: $T_{1/2}^{215}\text{Po}$ is the radioactive half-life of ^{215}Po)	s
t_0	Counting time of the background by alpha spectrometry	s
t_1	Time elapsed between separation and counting	s
t_g	Sample counting time by alpha spectrometry	s
U	Expanded uncertainty	
u	Standard uncertainty	
u_{rel}^2	Relative uncertainty	
$u(c_A)$	Standard uncertainty of the activity concentration of ^{226}Ra	$\text{Bq}\cdot\text{l}^{-1}$
$\tilde{u}(\widetilde{c_A})$	Standard uncertainty of the estimator c_A as a function of an assumed true value $\widetilde{c_A}$ of the measurand	$\text{Bq}\cdot\text{l}^{-1}$
$\tilde{u}(c_A^\#)$	Standard uncertainty of an estimate of the measurand when the true value is equivalent to the detection limit	$\text{Bq}\cdot\text{l}^{-1}$
V	Sample volume	l
ω	Distribution function of the standardized normal distribution	
w	Estimate of the calibration factor	l^{-1}

If the results are expressed in mass activity, the symbol c_A is replaced by a and the volume (V) is replaced by the sample mass (m).

5 Principle

Radium-226 is a naturally occurring isotope from the ^{238}U decay series (Fig. 1). It has a half-life of $1\,600 \pm 7$ a.[9] Radium-226 decays through alpha emission to ^{222}Rn [9].

Figure 1 — ^{238}U decay seriesFigure 2 — ^{237}Np decay series

To determine ^{226}Ra in water, a water sample is collected, filtered, and acidified (see [Clause 6](#) on sampling and storage).

Radium-225 tracer is added to the sample via a solution of ^{229}Th in equilibrium with its progeny ^{225}Ra (see [Figure 2](#)). Enough tracer is added to obtain a good statistical precision and be easily distinguished from a blank sample (e.g. 15-30 mBq). Radium-225 is the preferred tracer for ^{226}Ra determination by alpha spectrometry, because it is usually not present in environmental samples. Note that other tracers can also be used. Radium-224 (from a ^{228}Th solution) and ^{223}Ra (from a ^{227}Ac solution) can also be used if no significant ^{224}Ra or ^{223}Ra activity is expected to be present in the sample. Also, ^{133}Ba can be used as a recovery tracer if it is proven that it behaves like ^{226}Ra . Barium-133 is measured by gamma spectrometry.