

American National Standard



ANSI/AAMI/ ISO 15223-1: 2022

Medical devices—Symbols
to be used with information
to be supplied by the
manufacturer—
Part 1: General requirements

Medical devices—Symbols to be used with information to be supplied by the manufacturer— Part 1: General requirements

Approved 21 December 2022 by
AAMI

Approved 9 January 2023 by
American National Standards Institute

Abstract: Specifies symbols used to express information supplied for a medical device. This document is applicable to symbols used in a broad spectrum of medical devices, that are available globally and need to meet different regulatory requirements. These symbols can be used on the medical device itself, on its packaging or in the accompanying information. The requirements of this document are not intended to apply to symbols specified in other standards.

Keywords: symbols, medical devices, packaging, information supplied by the manufacturer

AAMI Standard

This Association for the Advancement of Medical Instrumentation (AAMI) standard implies a consensus of those substantially concerned with its scope and provisions. The existence of an AAMI standard does not in any respect preclude anyone, whether they have approved the standard or not, from manufacturing, marketing, purchasing, or using products, processes, or procedures not conforming to the standard. AAMI standards are subject to periodic review, and users are cautioned to obtain the latest editions.

CAUTION NOTICE: This AAMI standard may be revised or withdrawn at any time. AAMI procedures require that action be taken to reaffirm, revise, or withdraw this standard no later than five (5) years from the date of publication. Interested parties may obtain current information on all AAMI standards by calling or writing AAMI.

All AAMI standards, recommended practices, technical information reports, and other types of technical documents developed by AAMI are *voluntary*, and their application is solely within the discretion and professional judgment of the user of the document. Occasionally, voluntary technical documents are adopted by government regulatory agencies or procurement authorities, in which case the adopting agency is responsible for enforcement of its rules and regulations.

Published by

AAMI
901 N. Glebe Road, Suite 300
Arlington, VA 22203
www.aami.org

© 2023 by the Association for the Advancement of Medical Instrumentation

All Rights Reserved

This publication is subject to copyright claims of ISO and AAMI. No part of this publication may be reproduced or distributed in any form, including an electronic retrieval system, without the prior written permission of AAMI. All requests pertaining to this draft should be submitted to AAMI. It is illegal under federal law (17 U.S.C. § 101, *et seq.*) to make copies of all or any part of this document (whether internally or externally) without the prior written permission of the Association for the Advancement of Medical Instrumentation. Violator's risk legal action, including civil and criminal penalties, and damages of \$100,000 per offense. For permission regarding the use of all or any part of this document, contact Copyright Clearance Center.

Printed in the United States of America

ISBN 978-1-57020-861-4

Contents

Page

Committee representation	iv
Background of ANSI/AAMI adoption of ISO 15223-1:2021	v
Foreword	vi
Introduction	vii
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 General requirements	7
5 Symbols	7
Annex A (informative) Guidance and examples of <i>symbol</i> use, including multiple <i>symbols</i>	26
Annex B (informative) Use of general prohibition <i>symbol</i> and negation <i>symbol</i>	32
Bibliography	33

Figures

Figure 1—Relationship of terms used to describe <i>information supplied by the manufacturer</i>	2
---	---

Tables

Table 1— <i>Symbols</i> to convey <i>medical device</i> information	8
---	---

Committee representation

Association for the Advancement of Medical Instrumentation

Symbols and Nomenclature for Medical Devices Working Group

The adoption of ISO 15223-1 as an American National Standard was initiated by the AAMI Symbols and Nomenclature for Medical Devices Working Group (AAMI QM-WG03). AAMI QM-WG03 provides input to the AAMI Quality Management and Corresponding General Aspects for Medical Devices Committee (AAMI QM), which is the responsible group for providing the U.S. input to the relevant group in ISO/TC 210. U.S. representatives from AAMI QM-WG03 and the Technical Advisory Group (TAG) played an active part in developing the ISO document.

At the time this document was published, the **AAMI Symbols and Nomenclature for Medical Devices Working Group** has the following members:

Chair: Jeffrey Eggleston

Members: Mary-Zane Addy, Becton Dickinson & Company
Charles Buehler, Olympus America Inc
Michelle Carenza, Getinge USA
Lindsay Carrabine, Design Science Group, LLC
Scott Colburn, FDA/CDRH
Lianna Colombo, Draeger Medical Systems Inc.
Kat Crowder, Baxter Healthcare Corporation
Jeffrey Eggleston, Medtronic Inc Campus
Leonard Eisner, Eisner Safety Consultants
Christine Flahive, Chris Flahive Associates
Gottlieb Glauninger, Eli Lilly & Company
Richard Granquist, NAMSA
Shannon Hoste, Agilis Consulting Group LLC
Joe Justice, West Pharmaceutical Services, Inc.
Kay Kuckewich-Taylor, Becton Dickinson & Company
Michael Kuhn, Spacelabs Healthcare
Dan LaBelle, Nonin Medical Inc
Larry Lugo, Lugo & Associates LLC
Denis Moloney, Boston Scientific Corporation
Nick Momcilovic, GE Healthcare
Susumu Nozawa, Siemens Healthineers
David Osborn, Philips
Rodney Patch, Johnson & Johnson
Roger Alan Peterson, Arthrex Inc
Mike Powers, Intermountain Healthcare CESS
Michael Rakauskas, AbbVie
Kate Stephany, Smiths Medical
Staci Stoller, LivaNova PLC
Daidi Zhong, Chongqing University

Alternates: Barb Atzenhoefer, NAMSA
Ralf Behrends, GE Healthcare
Sally Jacobs, LivaNova PLC
Pierre Kernizan, Getinge USA
Karl Kortepeter, Veterans Administration (VA) Central Office
Michael Marchlik, Owens & Minor
Michael McCauley, Abbott Laboratories
Roger Moldon, Spacelabs Healthcare
Bruce Reedstrom, Boston Scientific Corporation
Bradford Spring, Becton Dickinson & Company
Nicole Zuk, Siemens Healthineers

NOTE Participation by federal agency representatives in the development of this standard does not constitute endorsement by the federal government or any of its agencies.

Background of ANSI/AAMI adoption of ISO 15223-1:2021

As indicated in the foreword to the main body of this document (page vi), the International Organization for Standardization (ISO) is a worldwide federation of national standards bodies. The United States is one of the ISO members that took an active role in the development of this standard, which was developed by ISO/TC 210 to specify general requirements for symbols to be used with information to be supplied by medical device manufacturers

U.S. participation in ISO/TC 210 is organized through the U.S. Technical Advisory Group, AAMI QM, administered by the Association for the Advancement of Medical Instrumentation. Experts from the United States made a considerable contribution to this standard.

AAMI encourages its committees to harmonize their work with International Standards in the area of symbols to be used with information to be supplied by medical device manufacturers. Upon review of ISO 15223-1:2021, the U.S. TAG to ISO/TC 210 and the AAMI Symbols and Nomenclature for Medical Devices Working Group decided to adopt it verbatim, as a revision of ANSI/AAMI/ISO 15223-1:2016.

AAMI and ANSI procedures require that standards be reviewed and, if necessary, revised every five years to reflect technological advances that may have occurred since publication.

As used within the context of this document, “shall” indicates requirements strictly to be followed to conform to the recommended practice. “Should” indicates that among several possibilities, one is recommended as particularly suitable, without mentioning or excluding others, or that a certain course of action is preferred but not necessarily required, or that (in the negative form) a certain possibility or course of action should be avoided but is not prohibited.

“May” is used to indicate that a course of action is permissible within the limits of the standard. “Can” is used as a statement of possibility and capability. Finally, “must” is used only to describe “unavoidable” situations, including those mandated by government regulation.

NOTE Users of this standard are advised that this document is an AAMI identical adoption of an ISO document and that the following international conventions have been carried over to the AAMI publication:

- British English spelling (e.g. colour instead of color)
- Use of SI units (e.g. metres instead of feet, Celsius instead of Fahrenheit, etc.)
- Decimal comma instead of a decimal point (e.g. 1 000,15 instead of 1,000.15)

The concepts incorporated in this standard should not be considered inflexible or static. This standard, like any other, must be reviewed and updated periodically to assimilate progressive technological developments. To remain relevant, it must be modified as technological advances are made and as new data comes to light.

Suggestions for improving this standard are invited. Comments and suggested revisions should be sent to Standards Department, AAMI, 901 N. Glebe Road, Suite 300, Arlington, VA 22203.

NOTE Beginning with the ISO foreword on page vi, this American National Standard is identical to ISO 15223-1:2021.

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 210, *Quality management and corresponding general aspects for medical devices*, in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/CLC/JTC 3, *Quality management and corresponding general aspects for medical devices*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

This fourth edition cancels and replaces the third edition (ISO 15223-1:2016), which has been technically revised.

The main changes compared to the previous edition are as follows:

- addition of 20 *symbols* that were validated as per ISO 15223-2;
- addition of 5 symbols previously published in ISO 7000, ISO 7001 and IEC 60417^[16];
- deletion of the defined term "labelling";
- inclusion of defined terms from ISO 20417, ISO 13485 and ISO 14971;
- expansion of the examples given in [Annex A](#);
- information about European regulations has been moved to informative notes throughout.

A list of all parts in the ISO 15223 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

Medical device *manufacturers* and others in the supply chain must provide specific information on the *medical device* itself, as part of the packaging, or in the *accompanying information*. For simplicity and to avoid translation of text, this information can be provided as *symbols* that have a specific meaning. This document does not specify the information that needs to be provided, but does specify internationally recognized *symbols* for the provision of this specific information.

The *symbols* included in this document have been published in ISO 7000, ISO 7001, IEC 60417^[16] or have been subjected to a formal *symbol* validation process.

This document is intended to be used by *manufacturers* of *medical devices* who market products in countries where there are specific language requirements. These *symbols* allow for a consistent portrayal of information. It can also be used by consumers or end users of *medical devices* who draw their supplies from a number of sources and can have varied language capabilities.

In this document, the conjunctive “or” is used as an “inclusive or”; so a statement is true if any combination of the conditions is true.

Terms defined in [Clause 3](#) are shown in *italic type* throughout the document.

In this document, the following verbal forms are used:

- “shall” indicates a requirement;
- “should” indicates a recommendation;
- “may” indicates a permission;
- “can” indicates a possibility or a capability;
- “must” indicates an external constraint that is not a requirement of the document.

Information marked as “NOTE” is intended to assist the understanding or use of the document. “Notes to entry” used in Clause 3 provide additional information that supplements the terminological data and can contain provisions relating to the use of a term.

Symbols added during the revision of this document were placed at the end of the pertinent section of [Table 1](#) to preserve the numbering of existing *symbols* and facilitate easy referencing of existing *symbols* in other documents.

NOTE Numbers given in square brackets throughout the document refer to the Bibliography.

Medical devices—Symbols to be used with information to be supplied by the manufacturer—

Part 1: General requirements

1 Scope

This document specifies *symbols* used to express information supplied for a *medical device*. This document is applicable to *symbols* used in a broad spectrum of *medical devices*, that are available globally and need to meet different regulatory requirements.

These *symbols* can be used on the *medical device* itself, on its packaging or in the *accompanying information*. The requirements of this document are not intended to apply to *symbols* specified in other standards.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3166-1, *Codes for the representation of names of countries and their subdivisions — Part 1: Country code*

ISO 8601-1, *Date and time — Representations for information interchange — Part 1: Basic rules*

ISO 8601-2, *Date and time — Representations for information interchange — Part 2: Extensions*

ISO 15223-2, *Medical devices — Symbols to be used with medical device labels, labelling, and information to be supplied — Part 2: Symbol development, selection and validation*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>.
- IEC Electropedia: available at <http://www.electropedia.org/>.

3.1

accompanying information

information accompanying or *marked* on a *medical device* or accessory for the user or those accountable for the installation, use, processing, maintenance, decommissioning and disposal of the *medical device* or accessory, particularly regarding safe use

Note 1 to entry: The *accompanying information* shall be regarded as part of the *medical device* or accessory.

Note 2 to entry: The *accompanying information* can consist of the *label*, *marking*, *instructions for use*, technical description, installation manual, quick reference guide, etc.

Note 3 to entry: *Accompanying information* is not necessarily a written or printed document but could involve auditory, visual, or tactile materials and multiple media types (e.g., CD/DVD-ROM, USB stick, website).

Note 4 to entry: See [Figure 1](#).

Note 5 to entry: The *label* can include the information on the packaging of the medical device.

Note 6 to entry: e-documentation can include any or all types of information supplied by the manufacturer partially or entirely.

Note 7 to entry: Marketing information is also known as promotional material.

Note 8 to entry: There is guidance or rationale related to accompanying information in ISO 20417:2021,^[15] Annex A.

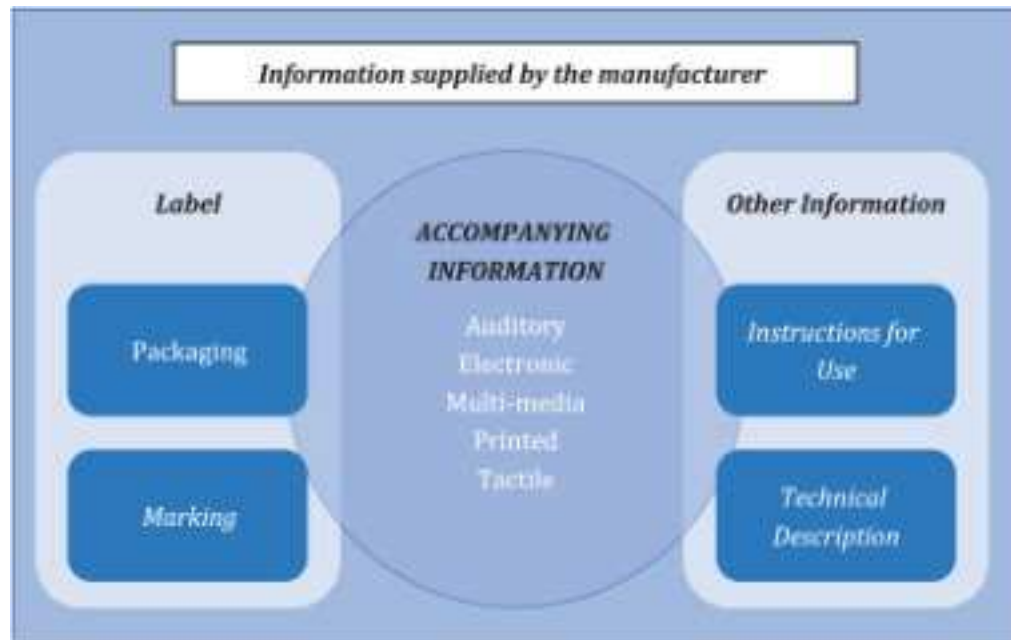


Figure 1—Relationship of terms used to describe *information supplied by the manufacturer*

[SOURCE: ISO 20417:2021,^[15] 3.2, modified — The following text has been removed from the graphic: “Scope of ISO 20417”, defined term reference numbers and a side box containing information outside the scope of ISO 20417. Note 8 to entry has been added.]

3.2

catalogue number

commercial product name

commercial product code

value given by the *manufacturer* to identify a specific *medical device* or accessory as it relates to its form/fit, function and process (i.e., manufacturing processes requiring differentiation for the end user)

Note 1 to entry: A *catalogue number* shall consist of letters or numbers or a combination of these.

Note 2 to entry: For the purposes of this document, *commercial product code* should not be confused with the US FDA, “product code” or procode classification.

Note 3 to entry: Synonyms for *catalogue number* are “reference number” or “reorder number”.

Note 4 to entry: See ISO 20417:2021, Figure 2.

[SOURCE: ISO 20417:2021,^[15] 3.3, modified — The cross-reference in Note 4 to entry has been revised to be external to this document.]

3.3

description

normative text which defines the purpose, the application and the use of the *symbol* (3.19)

[SOURCE: IEC 80416-1:2008, [\[19\]](#) 3.2, modified — “and optional product area” has been removed.]

3.4

distributor

natural or legal person, different from the manufacturer or *importer*, in the supply chain who, on their own behalf, furthers the availability of a *medical device* or accessory to the user

Note 1 to entry: More than one *distributor* may be involved in the supply chain.

Note 2 to entry: For the purposes of this document, persons in the supply chain involved in activities such as storage and transport on behalf of the *manufacturer*, *importer* or *distributor*, are not *distributors*.

Note 3 to entry: Distribution activities alone do not include repackaging or otherwise changing the container, wrapper, or *accompanying information* of the *medical device* or *medical device* package other than providing the identification of the *distributor*.

[SOURCE: ISO 20417:2021, [\[15\]](#) 3.5]

3.5

importer

natural or legal person who imports a *medical device* or accessory into a locale that was manufactured in another locale for the purposes of marketing

[SOURCE: ISO 20417:2021, [\[15\]](#) 3.8]

3.6

information supplied by the manufacturer

information related to the identification and use of a *medical device* or accessory, in whatever form provided, intended to ensure the safe and effective use of the *medical device* or accessory

Note 1 to entry: For the purposes of this document, e-documentation is included in *information supplied by the manufacturer*.

Note 2 to entry: For the purposes of this document, shipping documents and promotional material are excluded from *information supplied by the manufacturer*. However, some *authorities having jurisdiction* (defined in ISO 16142-1:2016, [\[9\]](#) 3.1) can consider such supplemental information as *information supplied by the manufacturer*.

Note 3 to entry: The primary purpose of *information supplied by the manufacturer* is to identify the *medical device* and its *manufacturer*, and provide essential information about its safety, performance, and appropriate use to the user or other relevant persons.

Note 4 to entry: See [Figure 1](#).

Note 5 to entry: There is guidance or rationale related to information supplied by the manufacturer in [Annex A](#).

[SOURCE: ISO 20417:2021, [\[15\]](#) 3.10, modified — The cross-reference in Note 2 to entry has been added. Note 5 to entry has been added.]

3.7

instructions for use

IFU

package insert

portion of the *accompanying information* that is essential for the safe and effective use of a *medical device* or accessory directed to the user of the *medical device*

Note 1 to entry: For the purposes of this document, a user can be either a lay user or professional user with relevant specialized training.

Note 2 to entry: For the purposes of this document, instructions for the professional processing between uses of a *medical device* or accessory can be included in the *instructions for use*.

Note 3 to entry: *The instructions for use*, or portions thereof, can be located on the display of a *medical device* or accessory.

Note 4 to entry: *Medical devices* or accessories that can be used safely and effectively without *instructions for use* are exempted from having *instructions for use* by some authorities with jurisdiction.

Note 5 to entry: See [Figure 1](#).

[SOURCE: ISO 20417:2021, ^[15] 3.11]

3.8

label

<*medical device*, accessory> written, printed or graphic information appearing on the item itself, on the packaging of each item, or on the packaging of multiple items

Note 1 to entry: For the purposes of this document, the term *labelled* is used to designate the corresponding act.

Note 2 to entry: *Label* includes the *marking* on the *medical device* or accessory.

Note 3 to entry: For the purposes of this document, information indicated on a graphical user interface (GUI) is considered as appearing on the item.

Note 4 to entry: See [Figure 1](#).

[SOURCE: ISO 20417:2021, ^[15] 3.12]

3.9

lot number

batch code

batch number

lot code

production control containing a combination of letters or numbers associated with a single lot or batch

Note 1 to entry: The title of *symbol* 5.1.5 uses the synonym *batch code*.

[SOURCE: ISO 20417:2021, ^[15] 3.15, modified — Note 1 to entry has been added.]

3.10

manufacturer

natural or legal person with responsibility for the design or manufacture, or both, of a *medical device* with the intention of making the *medical device* available for use, under his or her name; whether or not such a *medical device* is designed or manufactured, or both, by that person themselves or on their behalf by another person(s)

Note 1 to entry: The natural or legal person has ultimate legal responsibility for ensuring compliance with all applicable regulatory requirements for the *medical devices* in the countries or jurisdictions where it is intended to be made available or sold, unless this responsibility is specifically imposed on another person by the Regulatory Authority (RA) within that jurisdiction.

Note 2 to entry: The *manufacturer's* responsibilities are described in other GHTF guidance documents. These responsibilities include meeting both pre-market requirements and post-market requirements, such as adverse event reporting and notification of corrective actions.

Note 3 to entry: "Design or manufacture, or both", may include specification development, production, fabrication, assembly, processing, packaging, repackaging, labelling, relabelling, sterilization, installation, or remanufacturing of a *medical device*; or putting a collection of devices, and possibly other products, together for a medical purpose.

Note 4 to entry: Any person who assembles or adapts a *medical device* that has already been supplied by another person for an individual patient, in accordance with the *instructions for use*, is not the *manufacturer*, provided the assembly or adaptation does not change the intended use of the *medical device*.

Note 5 to entry: Any person who changes the intended use of, or modifies, a *medical device* without acting on behalf of the original *manufacturer* and who makes it available for use under his own name, should be considered the *manufacturer* of the modified *medical device*.

Note 6 to entry: An authorized representative, *distributor* or *importer* who only adds its own address and contact details to the *medical device* or the packaging, without covering or changing the existing labelling, is not considered a *manufacturer*.

Note 7 to entry: To the extent that an accessory is subject to the regulatory requirements of a *medical device*, the person responsible for the design, manufacture, or both, of that accessory is considered to be a *manufacturer*.

[SOURCE: ISO 14971:2019, [9](#) 3.9]

3.11

marking

information, in text or graphical format, durably affixed, printed, etched (or equivalent) to a *medical device* or accessory

Note 1 to entry: For the purposes of this document, the term *marked* is used to designate the corresponding act.

Note 2 to entry: For the purposes of this document, *marking* is different from “direct *marking*” as commonly described in unique device identification (UDI) standards and regulations. A UDI “direct *marking*” is a type of *marking*.

Note 3 to entry: See [Figure 1](#).

[SOURCE: ISO 20417:2021, [15](#) 3.16]

3.12

medical device

instrument, apparatus, implement, machine, appliance, implant, reagent for in vitro use, software, material or other similar or related article, intended by the *manufacturer* to be used, alone or in combination, for human beings, for one or more of the specific medical purpose(s) of:

- diagnosis, prevention, monitoring, treatment or alleviation of disease;
- diagnosis, monitoring, treatment, alleviation of or compensation for an injury;
- investigation, replacement, modification, or support of the anatomy or of a physiological process;
- supporting or sustaining life;
- control of conception;
- disinfection of *medical devices*;
- providing information by means of in vitro examination of specimens derived from the human body;

and does not achieve its primary intended action by pharmacological, immunological or metabolic means, in or on the human body, but which may be assisted in its intended function by such means

Note 1 to entry: Products which may be considered to be *medical devices* in some jurisdictions but not in others include:

- disinfection substances;
- aids for persons with disabilities;
- devices incorporating animal or human tissues, or both;
- devices for in vitro fertilization or assisted reproduction technologies.

[SOURCE: ISO 13485:2016, [4](#) 3.11]

3.13

model number

model

letters, numbers or a combination of these assigned by a *manufacturer* to distinguish by function or type, a particular *medical device*, *accessory* or *medical device family* from another

Note 1 to entry: See ISO 20417:2021, Figure 2.