

AS 3778.5.3:2022
ISO 15769:2010



STANDARDS
Australia



Measurement of water flow in open channels

Part 5.3: Guidelines for the application of acoustic velocity meters using the Doppler and echo correlation methods (ISO 15769:2010, IDT)



AS 3778.5.3:2022

This Australian Standard ® was prepared by CE-024, Measurement Of Water Flow In Open Channels and Closed Conduits. It was approved on behalf of the Council of Standards Australia on 19 May 2022.

This Standard was published on 10 June 2022.

The following are represented on Committee CE-024:

- Australian Bureau of Meteorology
- Australian Hydrographers Association
- Australian Industry Group
- Department of Planning, Industry and Environment, NSW
- Engineers Australia
- Institute of Instrumentation, Control & Automation Australia
- Irrigation Australia
- Joint Accreditation System of Australia & New Zealand
- National Measurement Institute
- Water NSW

This Standard was issued in draft form for comment as DR AS 3778.5.3:2022.

Keeping Standards up-to-date

Ensure you have the latest versions of our publications and keep up-to-date about Amendments, Rulings, Withdrawals, and new projects by visiting:

www.standards.org.au

ISBN 978 1 76113 808 9

Measurement of water flow in open channels

Part 5.3: Guidelines for the application of acoustic velocity meters using the Doppler and echo correlation methods (ISO 15769:2010, IDT)

Originated as AS 3778.5.3—2007.
Second edition 2022.

COPYRIGHT

© ISO 2022 — All rights reserved
© Standards Australia Limited 2022

All rights are reserved. No part of this work may be reproduced or copied in any form or by any means, electronic or mechanical, including photocopying, without the written permission of the publisher, unless otherwise permitted under the Copyright Act 1968 (Cth).

Preface

This Standard was prepared by the Standards Australia Committee CE-024, Measurement of water flow in open channels and closed conduits, to supersede AS 3778.5.3—2007, *Measurement of water flow in open channels, Part 5.3: Liquid flow in open channels and partly filled pipes—Guidelines for the application of Doppler-based flow measurements*.

The objective of this document is to provide guidelines on the principles of operation and the selection and use of Doppler-based and echo correlation velocity meters for continuous-flow gauging.

This document is applicable to channel flow determination in open channels and partially filled pipes using one or more meters located at fixed points in the cross-section.

This document is identical with, and has been reproduced from, ISO 15769:2010, *Hydrometry — Guidelines for the application of acoustic velocity meters using the Doppler and echo correlation methods*.

As this document has been reproduced from an International document, the following apply:

- (a) In the source text “this International Standard” should read “this document”.
- (b) A full point substitutes for a comma when referring to a decimal marker.

Australian or Australian/New Zealand Standards that are identical adoptions of international normative references may be used interchangeably. Refer to the online catalogue for information on specific Standards.

The terms “normative” and “informative” are used in Standards to define the application of the appendices or annexes to which they apply. A “normative” appendix or annex is an integral part of a Standard, whereas an “informative” appendix or annex is only for information and guidance.

Contents

Preface	ii
Foreword	v
1 Scope	1
2 Normative references	1
3 Terms, definitions and abbreviated terms	1
3.1 Terms and definitions	1
3.2 Abbreviated terms	3
4 Principles of operation of the techniques	3
4.1 Ultrasonic Doppler	3
4.2 Operating techniques	5
4.2.1 Introduction	5
4.2.2 Continuous wave Dopplers	5
4.2.3 Pulse incoherent	5
4.2.4 Pulse-to-pulse coherent	5
4.2.5 Spread spectrum (broad band)	6
4.2.6 Range gating	6
4.3 Bed-mounted Doppler systems	6
4.4 Side-looking/horizontal ADCPs	6
4.5 Acoustic (echo) correlation method	8
4.6 Velocity-index ratings	11
5 Factors affecting operation and accuracy	12
5.1 General	12
5.2 Characteristics of the instrument	12
5.2.1 Introduction	12
5.2.2 Ultrasonic beam angle (continuous wave Dopplers)	12
5.2.3 Beam “width”	14
5.2.4 Ultrasonic frequency	14
5.2.5 Method of determining velocity of sound	14
5.2.6 Signal processing	15
5.2.7 Instrument position and portion of the cross-section sampled	15
5.3 Channel and water characteristics	16
5.3.1 Channel geometry	16
5.3.2 Depth	18
5.3.3 Reflector density and efficiency	18
5.3.4 Homogeneity	18
5.3.5 Velocity of sound	19
5.3.6 Bed-mounted devices: siltation, sensor position	19
5.3.7 Significance of water level uncertainty	21
5.4 Effect of weed	21
6 Site selection	21
6.1 General	21
6.2 General site requirements for Dopplers and echo correlation devices	21
6.3 Bed-mounted ultrasonic Doppler and echo correlation devices	22
6.4 Side-lookers	23
7 Measurements	23
7.1 Velocity	23
7.1.1 Ultrasonic Dopplers (bed mounted)	23
7.1.2 Ultrasonic Dopplers (H-ADCPs/side-lookers)	23
7.1.3 Echo correlation	23
7.2 Water level	24
7.3 Determination of cross-sectional area	24

8	Installation, operation and maintenance	25
8.1	Installation considerations	25
8.1.1	General	25
8.1.2	Bed-mounted instruments	25
8.1.3	H-ADCPs/side-lookers	26
8.2	General maintenance considerations	26
9	Calibration, evaluation and verification	27
9.1	General	27
9.2	Calibration and performance checking	28
9.2.1	General	28
9.2.2	Indexing method	28
9.2.3	Performance checking	28
10	Determination of discharge	28
10.1	General	28
10.2	Velocity-index ratings	29
10.2.1	General	29
10.2.2	Determination of mean velocity from calibration data	30
10.2.3	Distribution of velocity in open channels	31
10.2.4	Forms of velocity-index ratings	31
11	Uncertainties in discharge determinations	33
11.1	General	33
11.2	Definition of uncertainty	33
11.3	General expectations of performance	34
11.4	Methodology of estimating the uncertainty in discharge determination	35
11.4.1	Sources of uncertainty	35
11.4.2	Determination of the uncertainty in the velocity-index rating	36
11.4.3	Uncertainty in the stage	36
11.4.4	Overall uncertainty	37
11.4.5	Uncertainty — Example of uncertainty estimation	37
11.4.5.1	Introduction	37
11.4.5.2	Uncertainty in the measured velocity u_{VI}	38
11.4.5.3	Uncertainty in velocity-index rating u_{Vr}	38
11.4.5.4	Uncertainty in the stage measurement u_h	38
11.4.5.5	Uncertainty in the cross-sectional area u_{Ar}	39
11.4.5.6	Uncertainty budget	39
11.4.5.7	Overall uncertainty U_Q	39
12	Points to consider when selecting equipment	39
Annex A	(informative) Selection considerations for ultrasonic Doppler and echo correlation devices	41
Annex B	(informative) Practical considerations	43
Annex C	(informative) Introduction to measurement uncertainty	47
Annex D	(informative) Performance guide for hydrometric equipment for use in technical standards	55
Annex E	(informative) Sample questionnaire — Doppler- and echo-correlation-based flowmeters	57
Bibliography		62

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 15769 was prepared by Technical Committee ISO/TC 113, *Hydrometry*, Subcommittee SC 1, *Velocity area methods*.

This first edition of ISO 15769 cancels and replaces ISO/TS 15769:2000, which has been technically revised.

NOTES

Australian Standard®

Measurement of water flow in open channels

Part 5.3: Guidelines for the application of acoustic velocity meters using the Doppler and echo correlation methods (ISO 15769:2010, IDT)

1 Scope

This International Standard provides guidelines on the principles of operation and the selection and use of Doppler-based and echo correlation velocity meters for continuous-flow gauging.

This International Standard is applicable to channel flow determination in open channels and partially filled pipes using one or more meters located at fixed points in the cross-section.

NOTE A limitation of the techniques is that measurement is made of the velocity of particles, other reflectors or disturbances.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document applies.

ISO/TS 25377:2007, *Hydrometric uncertainty guidance (HUG)*

ISO 772, *Hydrometry — Vocabulary and symbols*

3 Terms, definitions and abbreviated terms

3.1 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 772 and the following apply.

3.1.1

beam angle

mounting angle of the acoustic transducer relative to the normalized profiling direction

Note 1 to entry: Different beam angles will be suitable for different applications.

3.1.2

beam width

width of the acoustic signal transmitted, in degrees (°), from the centre of the transducer

Note 1 to entry: This, coupled with the side lobe of the acoustic signal, will affect the suitability of a particular instrument for its application, based on the mounting location and the distance of the water volume measured from the sensor.

3.1.3

bed-mounted device

upward-looking Doppler or echo correlation device that measures velocities within a beam looking upwards at an angle through the water column

3.1.4**bin
depth cell**

portion of the water sampled by the instrument at a known distance and orientation from the transducers

Note 1 to entry: The instrument determines the velocity in each cell.

3.1.5**blanking distance**

portion of water close to the instrument that is not sampled by Doppler technology

Note 1 to entry: This is left blank to allow the transducer to stop “ringing” before it receives reflected signals.

Note 2 to entry: It is also used to avoid the instrument sampling velocity in the zone of flow interference created close to, and by, the instrument.

3.1.6**broad-band Doppler**

instrument that records velocity at set distances from the sensor (see range-gated Doppler, 3.1.11) using coded acoustic pulses to make multiple velocity measurements from a single pulse pair (ping)

3.1.7**continuous Doppler**

simple type of Doppler instrument that measures the Doppler shift of all the particles within the range of the beam, taking the frequency with the largest peak as the average

3.1.8**downward-looking device**

instrument that can be deployed floating on the water surface looking down into the water column

3.1.9**echo (cross) correlation**

acoustic technique for recognizing echo images that can be used to determine the velocity of particles moving in the flowing water

3.1.10**profiling Doppler**

Doppler instrument that discriminates between signals from reflectors at different distances from the sensor and uses this information to moderate the estimate of average velocity

3.1.11**range-gated Doppler**

sophisticated Doppler instrument that records particle velocities at pre-set distances from the sensor

Note 1 to entry: Some instruments can produce velocity profiles along the length of the beam, while others just log measurements from one or more pre-defined cells.

3.1.12**side lobe**

most transducers that are developed using current technology have parasitic side lobes that are emitted off the main acoustic beam

Note 1 to entry: The side-lobe effect needs to be allowed for in the design and operation of the instrument.

3.1.13**side-looker**

Doppler usually mounted on the side of the channel

3.1.14**stage**

water level measured relative to a fixed datum

EXAMPLE The level of the lowest point in the channel.

3.1.15

upward-looking device

bed-mounted instrument that looks up through the water column

3.2 Abbreviated terms

Abbreviation	Meaning	Notes
ADCP	acoustic Doppler current profiler	
ADP	acoustic Doppler profiler	This is a registered trademark of Sontek/YSI. ¹⁾
ADVM instrument	acoustic Doppler velocity meter	Term used to describe a profiling acoustic Doppler velocity.
ADVP	acoustic Doppler velocity profiler	Alternative acronym and name for ADCP.
H-ADCP	horizontal ADCP	Side/bank-mounted acoustic Doppler velocity profiler.
H-ADVM	horizontal ADVM	Side/bank-mounted acoustic Doppler velocity meter.

¹⁾ Sontek/YSI is an example of a suitable product available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of this product.

4 Principles of operation of the techniques

4.1 Ultrasonic Doppler

The method of velocity measurement used is based upon a phenomenon first identified by Christian Doppler in 1843. The principle of “Doppler shift” describes the difference, or shift, which occurs in the frequency of emitted sound waves as they are reflected back from a moving body.

The sensors of Doppler systems normally contain a transmitting and a receiving device (see [Figure 1](#)). A sound wave of high frequency (F_s) is transmitted into the flow of water and intercepted and reflected back at a different frequency by tiny particles or air bubbles (reflectors). A typical reflector n produces a frequency shift F_{dn} . The “shift” between transmitted and reflected frequencies is proportional to the movement of particles relative to the position of the sound source (i.e. the sensor).

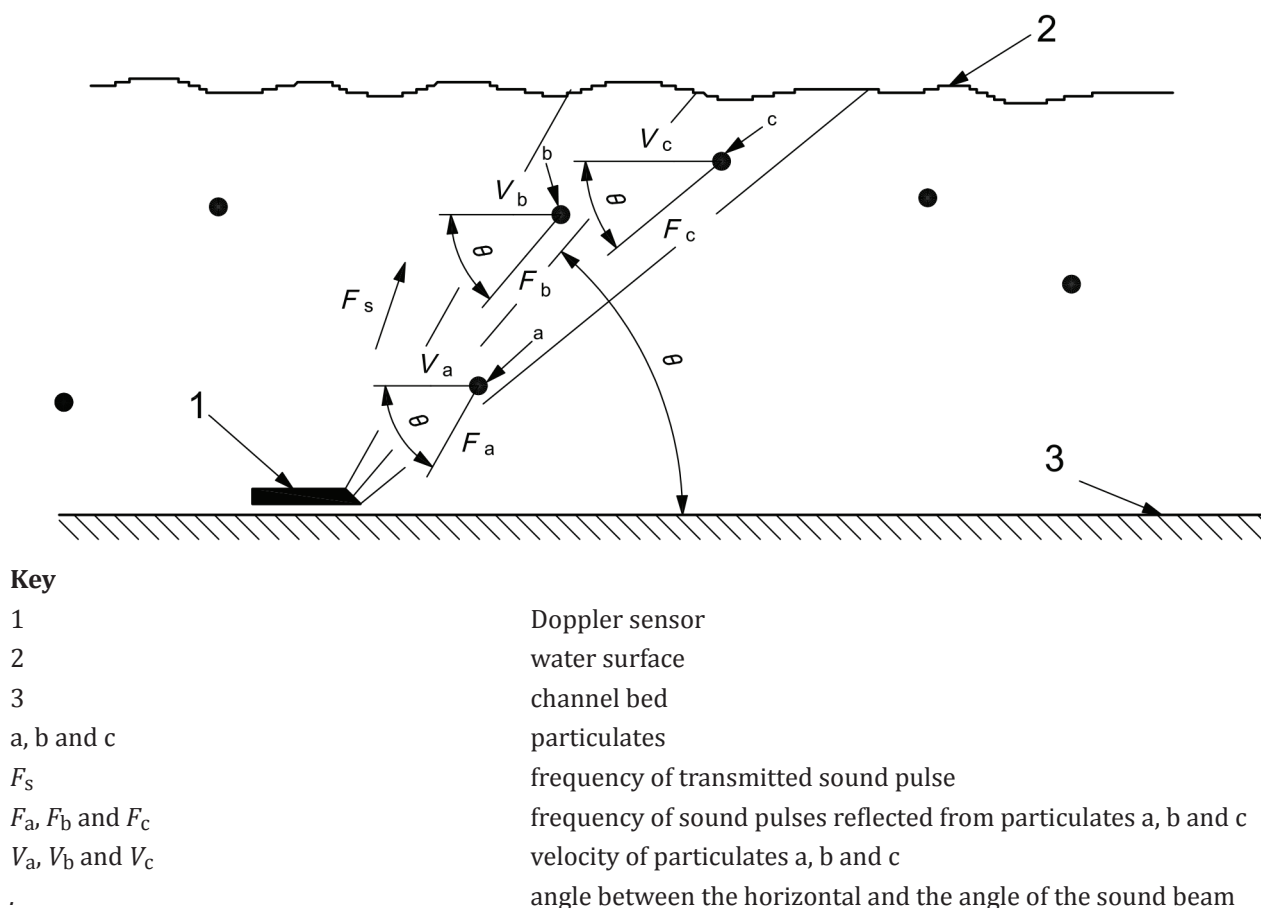


Figure 1 — Principle of Doppler ultrasonic flow measurement

Doppler shift only occurs if there is relative movement between the transmitted sound source and the reflected sound source along the acoustic beam (but not if it is perpendicular to it). The velocity of the moving reflector n can be calculated from

- the magnitude of the Doppler shift,
- the angle between the transmitted beam and the direction of movement, and
- the velocity of sound in water.

It can be shown that

$$v_n = F_{dn} \cdot c / 2F_s \cos \cdot n$$

where

F_{dn}	is the Doppler frequency shift produced by reflector n ;
F_s	is the frequency of sound with no movement;
v_n	is the relative velocity between the transmitted sound source and reflector n ;
c	is the velocity of sound in water;
$\cdot n$	is the angle between the reflector's line of motion (the assumed flow path) and the direction of the acoustic beam.

A Doppler velocity meter measures the resultant frequency shift produced by a large number of reflectors, of which reflector n is typical, and from that computes a mean velocity. It is the velocity of moving particles, and not water velocity, which is measured. By including the velocity of many particles,

it aims to make an estimate of the mean water velocity of the volume sampled by the acoustic beam. Although the particles, if small, will travel at almost the same speed as the water, sampling errors may occur depending on the spatial and velocity distribution of the particles.

The cross-sectional area is also required to apply the velocity-area calculation of discharge. Most systems incorporate a water-level sensor, and combining the water depth with knowledge of the cross-sectional profile allows the flow to be calculated.

4.2 Operating techniques

4.2.1 Introduction

All Dopplers fit into one of four general categories, based upon the method by which the measurements are made:

- a) continuous wave Dopplers;
- b) pulsed incoherent profiling Dopplers (including narrow band);
- c) pulse-to-pulse coherent;
- d) spread spectrum or broad band.

The last three of these four categories are all range gated. Range gating breaks the signal into successive segments and processes each segment independently of the others. This allows the instrument to measure the profile of the velocity at different distances from the instrument, with precise knowledge of the location of each velocity measurement. Reference should be made to the manufacturer's instrument manual to determine the type of instrument in use.

4.2.2 Continuous wave Dopplers

Pulse incoherent or continuous Dopplers are the simplest type of Doppler system. A continuous Doppler transmits a continuous signal with one transducer, while receiving the reflected signal with a separate transducer. The instrument measures the Doppler shift, which is used to calculate the velocity of the particles along the path of the acoustic beam. The instrument takes an average of the measured velocities calculated from the frequency and the strength of the loudest reflected signals. The instrument cannot determine the precise location within the water column. In some situations, this simplicity does not cause any problems but, in channels where the sediment distribution is uneven, the loudest signal may not represent the average velocity in the channel. In addition, in channels with a heavy sediment load, most of the signal would be reflected back before fully penetrating the water column. Thus, the loudest signal would be from close to the instrument and would not be representative of the average velocity in the channel.

4.2.3 Pulse incoherent

Incoherent Doppler or profiling systems are more sophisticated than continuous wave Dopplers, in that they take into account the distance travelled by the reflected signals when calculating the average velocity. An incoherent Doppler transmits a single pulse of sound and measures the Doppler shift, which is used to determine the velocity of the particles along the path of the acoustic beam. Based upon the elapsed time since the pulse was transmitted, and the speed of sound in water, the exact location of the velocity measurement is known. By range gating the return signal at different times, the profile of velocity with the distance away from the instrument can be determined.

4.2.4 Pulse-to-pulse coherent

Coherent Doppler systems follow many of the same measurement principles as incoherent Doppler systems, but use a different method for determining the Doppler shift. Coherent systems transmit one relatively short pulse, record the return signal and then transmit a second short pulse, when the return

from the first pulse is no longer detectable. The instrument measures the phase differences between the two returns and uses this to calculate the Doppler shift. Signals too close to the instrument are rejected.

4.2.5 Spread spectrum (broad band)

Like coherent systems, broad-band Dopplers transmit two pulses and look at the phase change of the return from successive pulses. However, with broad-band systems, both acoustic pulses are within the profiling range at the same time. The broad-band acoustic pulse is complex, it has a code superimposed on the wave form. The code is imposed on the wave form by reversing the phase and creating a pseudo-random code within the wave form. This pseudo-random code allows many independent samples to be collected from a single sound pulse. Because of the complexity of the pulse, the processing is slower than in a narrow-band system. However, multiple independent samples are obtained from each ping.

4.2.6 Range gating


The range gating method breaks the signal into successive segments and processes each segment independently of the others. Side-looking/horizontal ADCPs use this approach, as do several of the more sophisticated bed-mounted devices.

4.3 Bed-mounted Doppler systems

Bed-mounted Doppler systems include all four types of Doppler instrument. They are normally used in smaller channels, for example up to 5 m wide and 5 m deep, where they are often practical and easy to install. However, this does not mean they cannot be used in larger channels, even though it may be difficult to install bed-mounted instruments in particularly deep channels. If siltation is a problem, it may be possible to mount such devices on a raised platform or on the channel sides.

4.4 Side-looking/horizontal ADCPs


These instruments are usually fixed to the side of the channel and look across the channel to determine velocities in one horizontal layer across the full width, or a portion of the width, of the cross-section (excluding the blanking distance). Most systems consist of two transducers, one sending a beam diagonally across the channel in an upstream direction and the other diagonally across the channel in a downstream direction [see [Figures 2 a\)](#) and [2 b\)](#)]. A fixed, side-looking ADCP does not estimate velocity throughout the full channel cross-section. With a known orientation of the transducers, each beam can be divided into an equal number of cells or bins and the component average velocity in the x-, y- and resultant directions can be determined for each cell. An integrated cell will give an average velocity, or individual cell velocities can then be averaged to determine the index velocity/measured velocity for the sampled length for the full distance sampled, or by selecting cells for a portion of the length. The mean velocity in the x-direction, i.e. at right angles to the measuring cross-section or parallel with the assumed direction of flow, is usually used to derive the velocity-index rating. Effectively, the instrument looks at a single horizontal layer across the channel (see [Figure 3](#)). This layer is divided into one or more sample cells or bins and the average velocity is computed for each. The operator can usually select the size and position of these measurement cells.

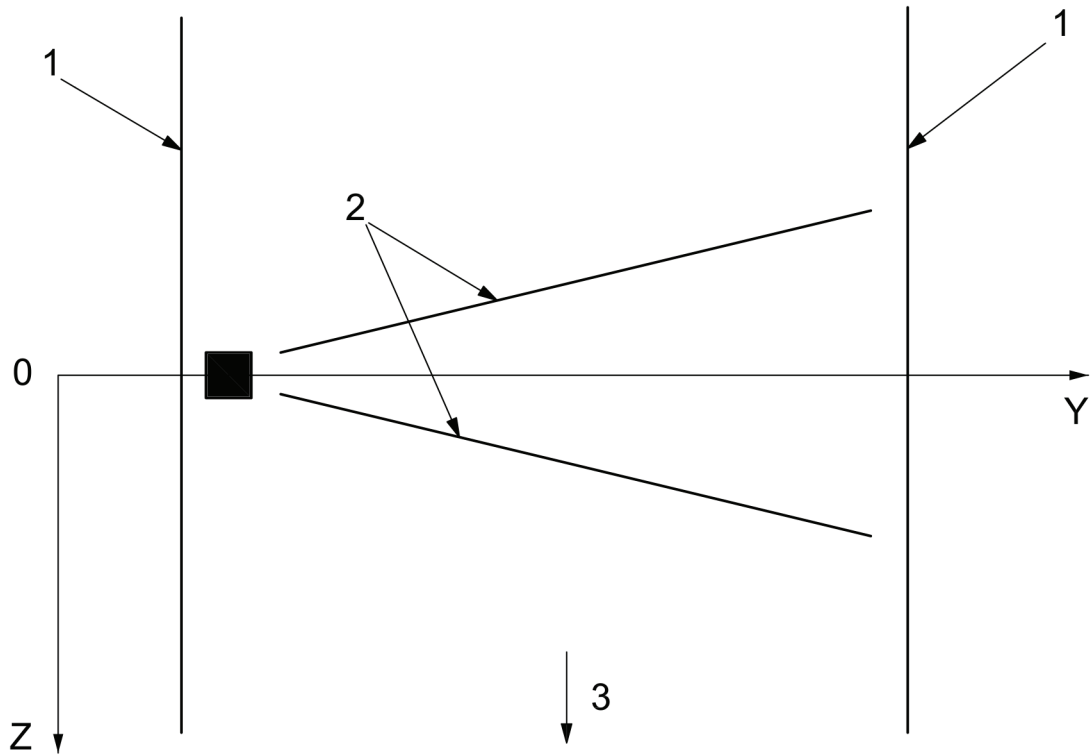

a) Plan view

Key


- 1 bank of channel
- 2 beams
- 3 direction of flow

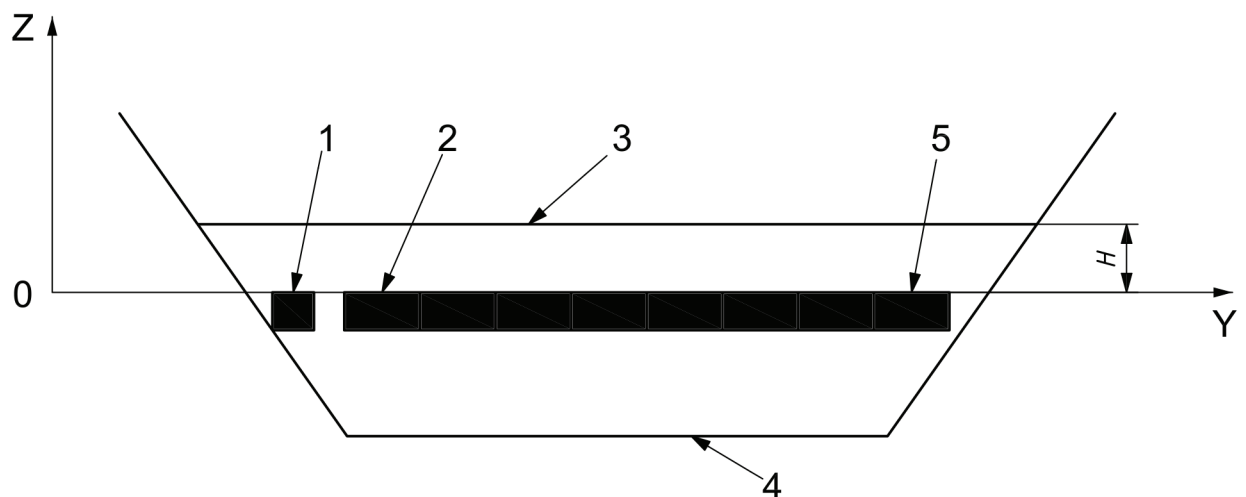

b) Side view

Key	
1	instrument
2	first cell
3	water surface
4	channel bed
5	last cell
H	height of water above cell

Figure 2 — Diagram illustrating a typical H-ADCP/side-looker beam and cell arrangement

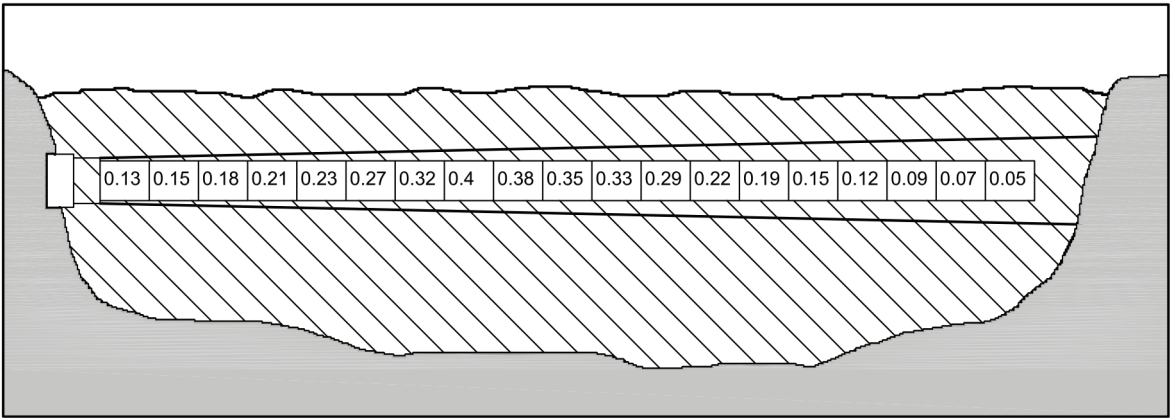

In this example, the beam is sampling the majority of the width of the channel. The average velocity in each cell is that averaged over the full beam width in the cell.

Figure 3 — Sketch illustrating the channel cross-section sampled by a side-looking ADCP, illustrating the spread of the beam, and the measurement cells sampled

Velocities close to the instrument typically remain unmeasured. This is for the following two reasons.

- a) The area near the transducer (blank after transmit) is left blank to allow the transducer to stop “ringing” before it receives reflected signals. The minimum blanking distance can be obtained from the manufacturer's literature.
- b) To avoid measuring in the zone of turbulence created by the instrument itself.

4.5 Acoustic (echo) correlation method

The echo (cross) correlation velocity meter is very similar to a bed-mounted ultrasonic Doppler in size and application. However, even though it is dependent on transmitted sound pulses being Doppler in size and application. However, even though it is dependent on transmitted sound pulses being reflected back from moving particles, it works on somewhat different principles. An ultrasonic transducer transmits a short ultrasonic pulse (or pulse code) into the water. These pulses are reflected by particles or air bubbles. The reflected ultrasonic echo from the first pulse is received as a characteristic pattern. This is digitized and stored as the first scan of the dated echo pattern. About 0,4 ms to 4 ms later, another ultrasonic pulse is transmitted and the incoming echo patterns are digitized and stored. This is the second scan pattern. Using the travel time difference between the transmission and reception time, the position of the particles in the flow cross-section can be determined. By means of cross-correlation, the echo patterns are checked within different time windows for agreement. The cross-correlation also delivers the temporal movement of the characteristic pattern in the second scan. This temporal movement of the pattern under consideration can be directly converted to the velocity of flow for this particular beam. The process is repeated a large number of times per second and single velocities at different distances are computed in real time. The instrument effectively divides the water column in

front of it into a number of cells, so it is possible to accurately determine the velocity profile in the vertical (see [Figures 4, 5 and 6](#)).

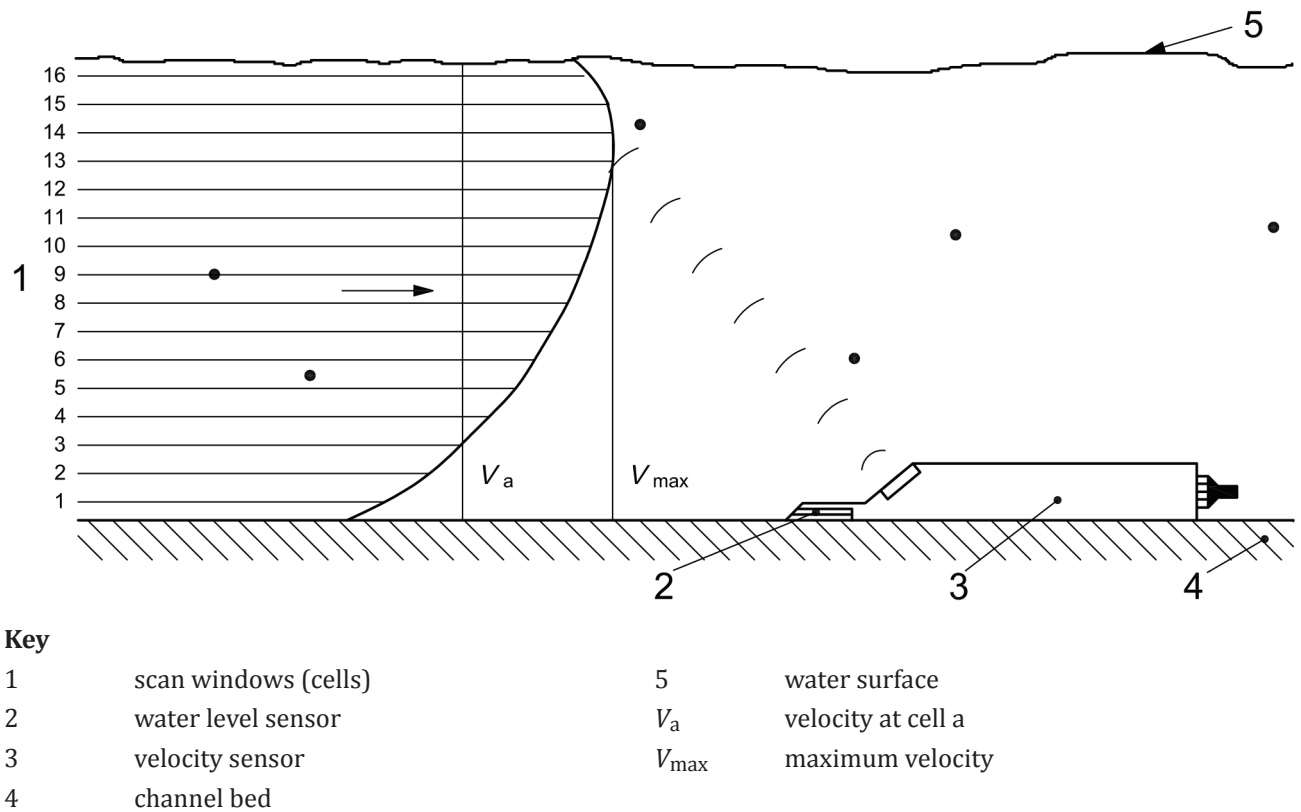
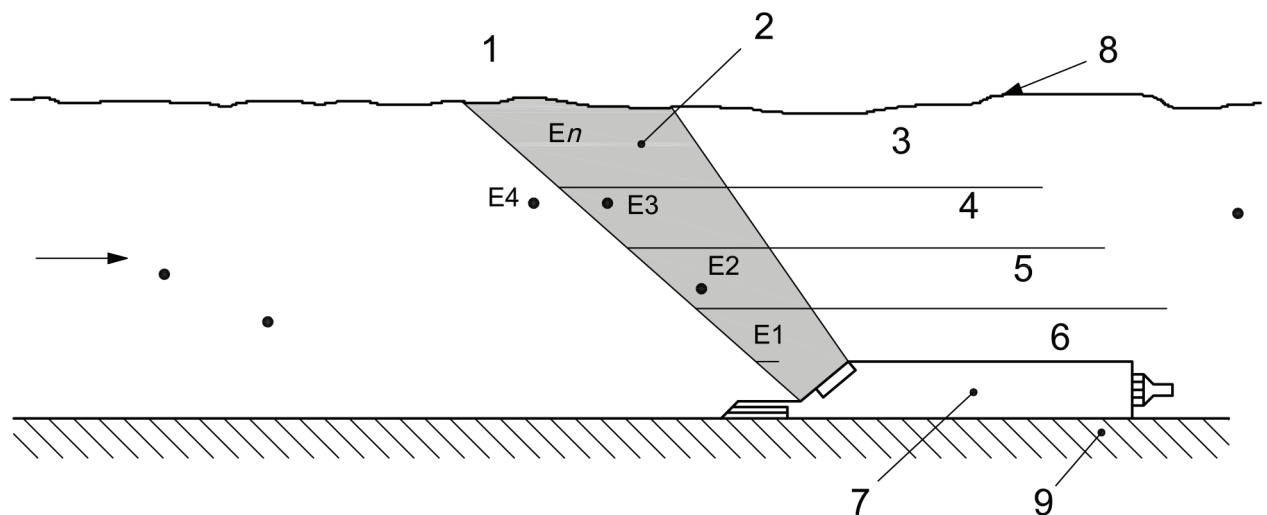


Figure 4 — Sketch illustrating an echo correlation velocity meter





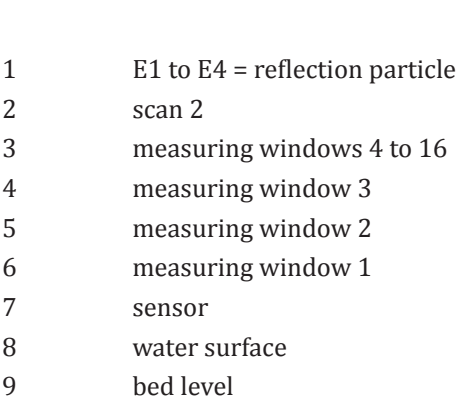


Figure 5 — Sketches illustrating the principles of the echo correlation velocity meter

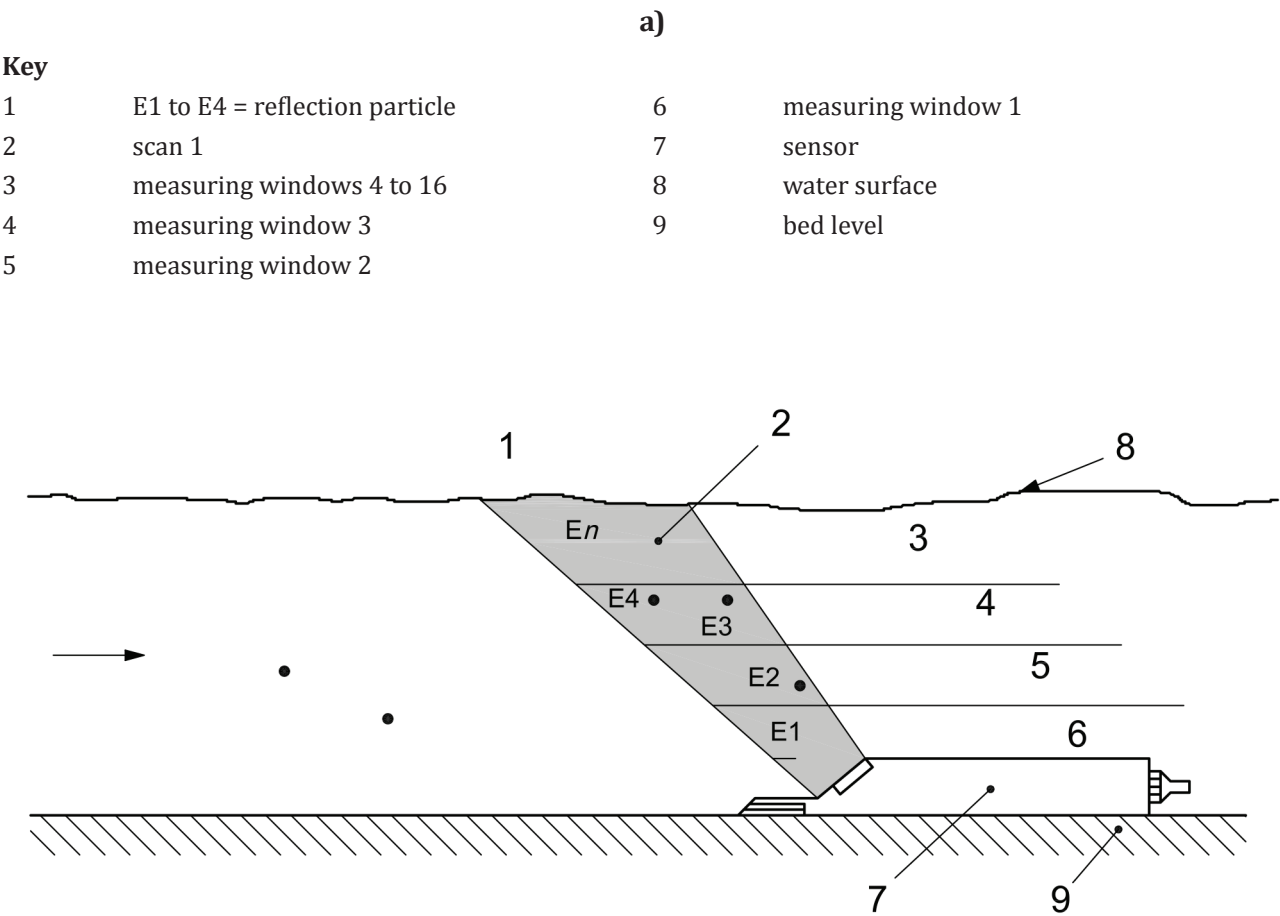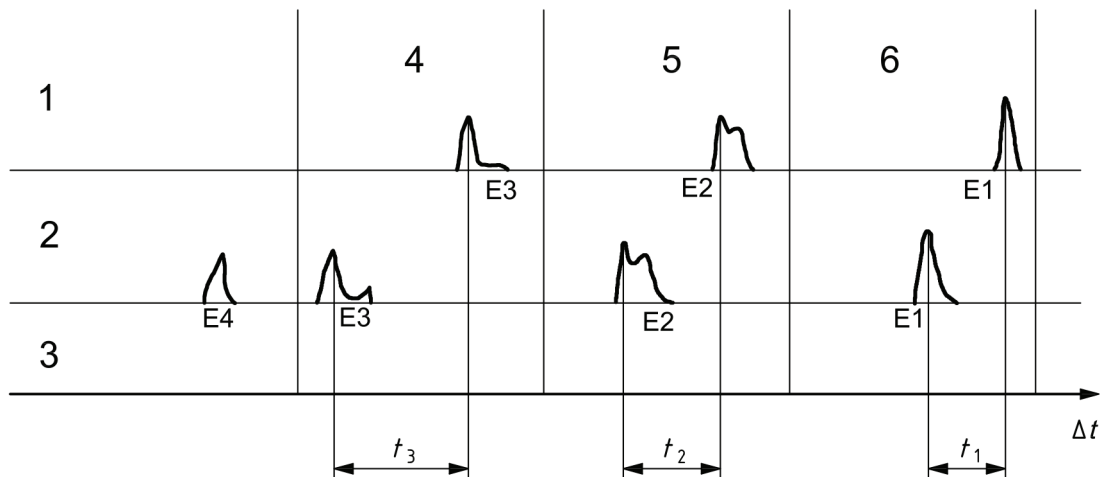

For n^{th} window: E_n is the echo in window n , t_n is the time between echoes in window n and n is the window number.

Key

1	signal reception, 1st scan	4	measuring window 3
2	signal reception, 2nd scan	5	measuring window 2
3	signal evaluation	6	measuring window 1

Figure 6 — Sketch illustrating the principles of the echo (cross) correlation technique

4.6 Velocity-index ratings

With the exception of multi-path transit-time ultrasonic systems with a significant number of operational paths (see ISO 6416), acoustic continuous-flow measuring devices require calibration. Unless the cross-section is relatively small, ultrasonic Doppler and echo correlation systems only measure velocity in part of the cross-section. By measuring the vertical profile, these devices obtain enough information that can be coupled with velocity distribution models to make a reasonable flow determination. As such, the measured velocity needs to be related to the mean velocity in the measuring section for any given stage and flow. A relationship between stage and cross-sectional area is also required. The relationship between mean cross-sectional velocity and the measured velocity (index velocity) is referred to as the velocity-index rating. Bottom-mounted, range-gated devices (that thus measure the vertical profile of velocity) can provide reasonable flow data without calibration in relatively small channels (<2 m to 3 m in width and depth) that are concrete lined with a regular (i.e. trapezoidal) cross-section. Nevertheless, even if the instrument can effectively sample velocity throughout the cross-section, verification gaugings are required to confirm that the discharge is being determined accurately.

In order to establish an index velocity relationship, independent measurements of discharge are made using an independent gauging method and the instrument velocities and stage readings are noted. The discharge obtained by gauging is divided by the cross-sectional area at the velocity-sensing device (obtained from the stage-area relationship), to obtain the mean velocity for that section. A relationship can then be derived to obtain the mean velocity from the measured velocity. The measured velocity is often referred to as the index velocity. There are two types of relationship that are commonly used:

- mean velocity = function (index velocity);
- mean velocity = function (index velocity, stage).

The former is used at sites where the relationship between mean velocity and measured velocity is relatively stable, whereas the latter is generally used at sites where the flow conditions vary with not only velocity, but also with stage. A reasonably intensive calibration effort is required to apply the indexing method.

5 Factors affecting operation and accuracy

5.1 General

The factors affecting the performance of Doppler and echo correlation velocity meters may be broadly divided into characteristics of the instrument and those of the channel or the liquid flowing in it. However, the effects interact and must be considered together.

In addition to the issues raised in [5.2](#) and [5.3](#), further practical considerations are highlighted in [Annex B](#).

5.2 Characteristics of the instrument

5.2.1 Introduction

The characteristics of the instrument and, in particular, the sensor, will have a bearing on its performance in any given situation. There is no optimum set of characteristics. Some environmental factors will make a particular instrument perform better under some conditions but worse under others.

5.2.2 Ultrasonic beam angle (continuous wave Dopplers)

For the simpler, continuous wave bed-mounted Doppler systems, the ultrasonic “beam” is usually transmitted in the approximate shape of a cone. The term “beam angle”, or “projection angle”, in this context, refers to the angle between the cone axis and the flow direction. This subclause describes the effects of beam angle, though in fact the beam “width” must be considered at the same time (see [5.2.3](#)). Range-gated/profiling Dopplers inherently use narrow band widths (typically 1,4° to 2,8°). Therefore, this subclause is mainly concerned with continuous wave Dopplers.

The sensor has to be installed so that it is below the liquid surface under all conditions of interest and in such a way that the beam cone reaches the lateral extremities of the channel as far as possible. The installed position is often a compromise and the installer is frequently obliged to install the sensor on the channel bed, somewhere near the centre of the cross-section. An off-centre position is sometimes used.

Assuming that an ultrasonic Doppler sensor is installed on the bed of the channel, a high angle between the flow direction and ultrasonic beam (for example between 30° and 50°) will enable signals to be obtained throughout the depth up to the limit of the penetration of the beam. However, no signals will be obtained close to the bed on either side of the sensor. Serious sampling errors will occur, particularly when the ratio between the depth of water and width of the channel is low [see [Figures 7 a\)](#) and [7 b\)](#)].

Conversely, a shallow beam angle will allow flow to be measured close to the bed and be best for shallow depths. However, a beam at a shallow angle may not reach the lateral extremities if the channel is too wide or not sufficiently long. In a long channel, the beam might theoretically reach the extremities but the penetration (range) of the beam may not be sufficient to do so [see [Figures 7 a\)](#) and [7 b\)](#)].

Beam “width” also has a bearing on the velocity sampling (see [5.2.3](#)).

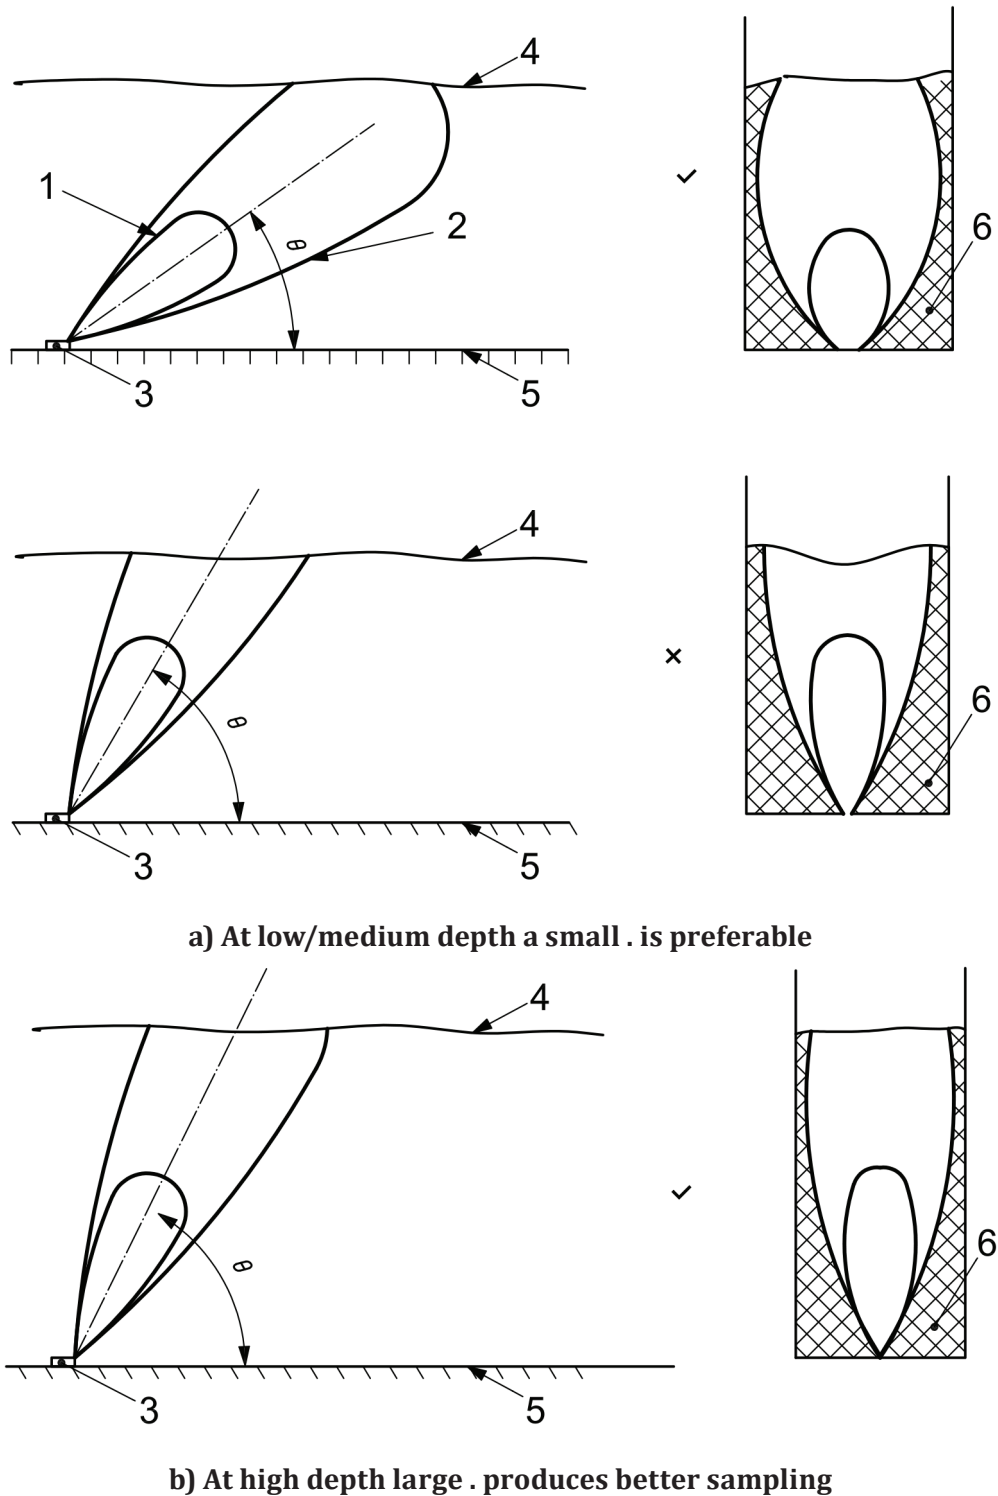


Figure 7 — Bed-mounted continuous wave Doppler beam angle effects

5.2.3 Beam “width”

Beam width is a loose term indicating the spread of the beam. It is a function of sound frequency and diameter of the transmitter. The designer of the instrument may be constrained by other factors in his scope to vary the beam width.

A wide beam, i.e. one with a cone having a large spread, will give best coverage in that signals will be obtained over a greater area of the channel. However, there will be an uncertainty in velocity measurement, since the wide beam means that the actual angle made by a particular reflector may be different from the mean beam angle assumed by the instrument. Furthermore, a bias could occur depending on the distribution of velocity and reflector concentration.

A narrow beam width would have less angular uncertainty but a poorer coverage (sampling). A narrow beam allows for a longer profiling distance (greater range). Side-lookers and other range-gated and profiling instruments tend to have narrow band widths. This allows the instrument to profile, across the channel, a greater distance before the beam spread strikes a boundary. This makes them far more suitable for use in larger rivers than continuous wave Doppler systems.

If the distribution of reflectors and velocity are both fairly uniform, sampling is unimportant and a narrow beam width would give best results because the uncertainty relating to beam angle is minimized. In contrast, if the velocity distribution is non-uniform, a wide beam width will give a better sample of velocity than a narrow one. If, at the same time, the reflector distribution is uniform, the error relating to beam angle may be acceptable and so a wide beam width will be preferable.

If neither the velocity profile nor the reflector density is uniform, a significant uncertainty of measurement can be expected whatever the beam width.

Care must be taken to ensure that the range (distance from the sensor) and beam width are taken into account to ensure that the acoustic beam is not hitting a surface, i.e. channel bed or water surface (see [5.2.7.3](#)).

5.2.4 Ultrasonic frequency

A lower frequency will generally penetrate further (greater range) but will require a larger transducer for a given beam width. A larger width/depth of channel will therefore benefit from a lower frequency transducer where the larger sensor size will not present a serious obstruction.

5.2.5 Method of determining velocity of sound

The velocity of sound in water varies with density, which is a function of temperature, salinity and pressure. Since the velocity of sound appears in the velocity determination formulae for Doppler-based instruments, errors will occur if no adjustment is made. Some instruments have no dynamic adjustment, though it is possible to put in a fixed calibration factor. This is acceptable provided the conditions do not change. Other instruments have a temperature sensor and a dynamic correction for temperature effects. This is acceptable for conditions where the water content is unchanging but the temperature does change.

When the temperature and salinity are variable, the only satisfactory solutions are for the instrument to measure the velocity of sound or to separately measure or estimate the temperature and salinity and to make a retrospective correction to the recorded data.

The effect of not making full or partial allowance for this variation is described in [5.2.6](#).