

STANDARDS AUSTRALIA/STANDARDS NEW ZEALAND

Amendment No. 1
to
AS/NZS 2430.3.6:2004
Classification of hazardous areas
Part 3.6: Examples of area classification—Laboratories, including fume cupboards
and flammable medical agents

CORRECTION

The 2004 edition of AS/NZS 2430.3.6 is amended as follows; the amendments should be inserted in the appropriate places.

SUMMARY: This Amendment applies to Clause 5.2.2 and Figure 5.1.

Published on 16 March 2007.

Approved for publication in New Zealand on behalf of the Standards Council of New Zealand on 23 February 2007.

Page 6 Clause 5.2.2

- 1 In the title of the Clause, *replace* 'AS/NZS 2248.8)' with AS/NZS 2243.8)'.
2 In point (c), *delete* '0.5 m' and *replace* with '1.5 m'.
-

Page 7 Figure 5.1

Delete Figure 5.1 and *replace* with the following:

AMDT
No. 1
MAR
2007

AMDT
No. 1
MAR
2007

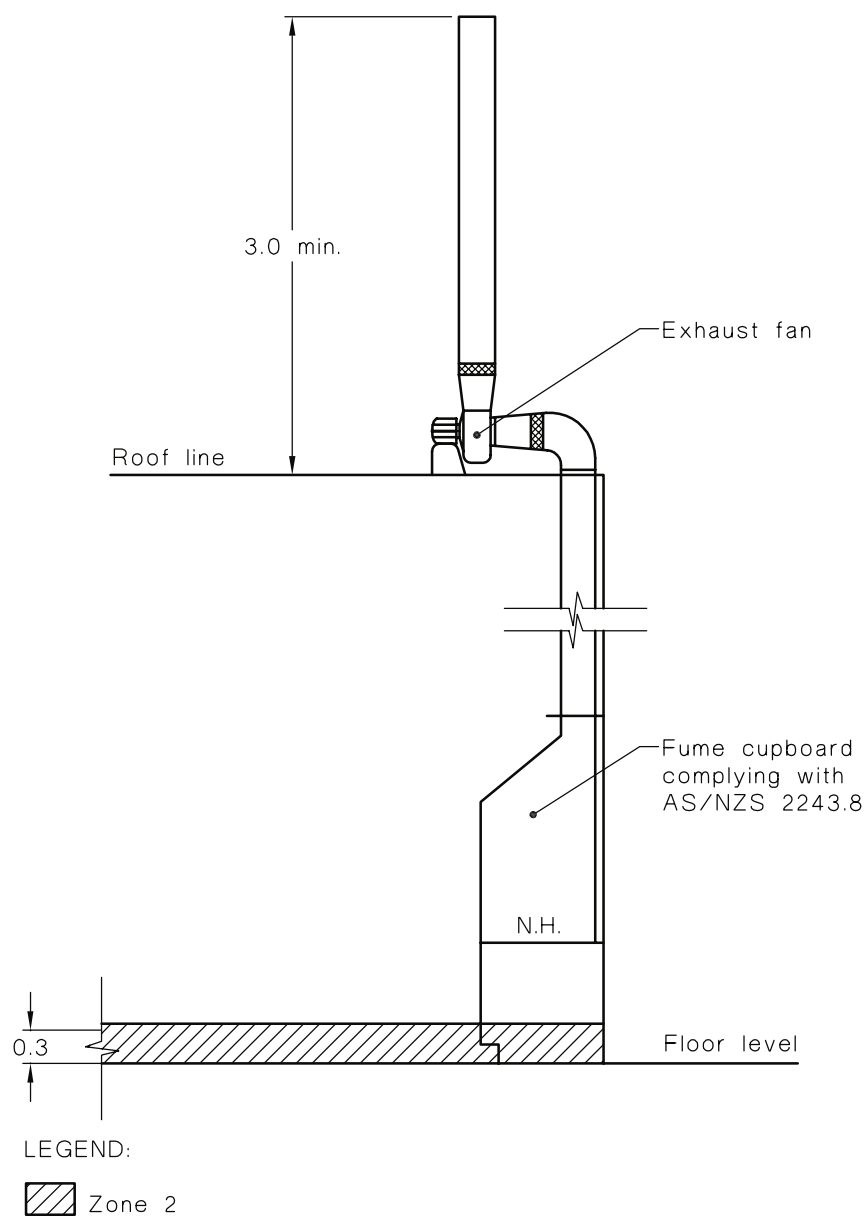


FIGURE 5.1 FUME CUPBOARD COMPLYING WITH AS/NZS 2243.8 AND LABORATORY FLOOR LEVEL