



Designation: D4230 – 20

Standard Test Method for Measuring Humidity with Cooled-Surface Condensation (Dew-Point) Hygrometer¹

This standard is issued under the fixed designation D4230; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers the determination of the thermodynamic dew- or frost-point temperature of ambient air by the condensation of water vapor on a cooled surface. For brevity, this is referred to in this test method as the condensation temperature.

1.2 This test method is applicable for the range of condensation temperatures from 60°C to –70°C.

1.3 This test method includes a general description of the instrumentation and operational procedures, including site selection, to be used for obtaining the measurements and a description of the procedures to be used for calculating the results.

1.4 This test method is applicable for the continuous measurement of ambient humidity in the natural atmosphere on a stationary platform.

1.5 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.6 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.* For specific precautionary statements, see Section 8.

1.7 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

2.1 *ASTM Standards:*²

D1356 Terminology Relating to Sampling and Analysis of Atmospheres

D3631 Test Methods for Measuring Surface Atmospheric Pressure

3. Terminology

3.1 *Definitions:*

3.1.1 For definitions of other terms in this test method, refer to Terminology D1356.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *nonhygroscopic material, n*—material that neither absorbs nor retains water vapor.

3.2.2 *mirror (front surface), n*—a polished surface, usually a metallic surface, on which condensates are deposited.

3.3 *Symbols:*

- e = vapor pressure of water vapor in moist air.
- e_i = saturation pressure of water vapor in equilibrium with the plane surface of ice.
- e_w = saturation pressure of water vapor in equilibrium with the plane surface of water.
- P = ambient pressure.
- r = mixing ratio.
- T = ambient air temperature.
- T_d = thermodynamic dew- or frost-point temperature.
- RH_i = relative humidity with respect to ice.
- RH_w = relative humidity with respect to water.

4. Summary of Test Method

4.1 The ambient humidity is measured with a dew- and frost-point hygrometer.

¹ This test method is under the jurisdiction of ASTM Committee D22 on Air Quality and is the direct responsibility of Subcommittee D22.11 on Meteorology.

Current edition approved March 1, 2020. Published April 2020. Originally approved in 1983. Last previous edition approved in 2012 as D4230 – 02 (2012). DOI: 10.1520/D4230-20.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

4.2 The mirror or some other surface on which the condensate is deposited is provided with the means for cooling and heating, detection of condensate, and the measurement of the temperature of the mirror surface.

4.3 Calculations of saturation vapor pressure over water and ice as functions of temperature are provided.

5. Significance and Use

5.1 Humidity information is important for the understanding of atmospheric phenomena and industrial processes. Measurements of the dew-point and calculations of related vapor pressures are important to quantify the humidity information.

6. Interferences

6.1 This test method is not applicable if other constituents in the atmosphere condense before water vapor.

7. Apparatus

7.1 *Dew-point hygrometers*, specifically designed for meteorological observations are available commercially. A schematic arrangement of a typical optical dew-point hygrometer is shown in Fig. 1.

7.1.1 The sample air flows through a small chamber.

7.1.2 Within the chamber is a mirror or surface on which the condensate can be deposited.

7.1.3 A beam of light from an incandescent lamp, light emitting diode or other suitable light source shines on the mirror.

7.1.4 Dew or frost is detected with an electro-optic device.

7.1.5 The mirror is cooled by a Peltier thermoelectric element. Peltier cooling is a convenient method for unattended and automatic instruments.

7.1.6 Preferred devices of sensing mirror temperature are resistance thermometers, thermistors, and thermocouples.

7.1.6.1 The temperature sensors shall be attached to or embedded in the mirror to measure the temperature of the surface of the mirror.

7.1.7 Suitable control circuitry shall be provided to maintain a constant quantity of condensate on the mirror.

7.1.8 Suitable provisions shall be provided to compensate for the contamination of the surface of the mirror.

7.2 Auxiliary Equipment:

7.2.1 Provision shall be provided for assuring air flow past the dewpoint mirror without changing the pressure in the mirror chamber more than 0.5 % from the ambient pressure surrounding the sensor. An air flow of approximately 1.1 litres per minute is recommended for typical chambers.

7.2.2 Readout instrumentation is available with the dew-point hygrometer.

8. Precautions

8.1 Safety Precautions:

8.1.1 The hygrometer shall be packaged in a suitable enclosure for application in industrial or outdoor environment.

8.1.2 Electrical connectors and cables shall be suitable for the industrial or outdoor environment.

8.1.3 Appropriate voltage surge protection circuitry must be incorporated.

8.2 Technical Precautions:

8.2.1 The accuracy of a cooled-surface condensation hygrometer is degraded by the presence of water-soluble materials. A mirror-cleaning schedule, consistent with the contamination rate, is necessary to maintain the initial calibration accuracy. The user must determine the required maintenance schedule for the specific site, by comparison of calibrations made before and after cleaning.

8.2.2 Caution in performing this test method should be taken if the indicated mirror temperature is between 0°C and -30°C. Below freezing, the initial formation of the condensate on the surface of a mirror may be either dew or frost. In the case of nonfiltered atmospheric air, the supercooled water usually does not persist long on a mirror surface and quickly changes to frost. The only positive method for determining the state of the condensate is by visual observation of the mirror surface.

8.2.2.1 The following illustrates the magnitude of the error involved when dew or frost is not differentiated: The saturation vapor pressure of supercooled water at -30°C corresponds to saturation vapor pressure of ice at -27.2°C; dew point of -20°C corresponds to frost point of -18.0°C; -10°C dew point corresponds to frost point of -8.9°C. (The frost point temperature is approximately 90 % of the dew-point temperature in degrees Celsius.)

8.2.3 A positive method for identifying the state of the condensate is to visually observe the condensate on the mirror with the aid of a microscope or other optical magnifier.

8.2.4 A finite length of time is required for the condensate to deposit on the mirror and for the hygrometer to reach equilibrium with the ambient humidity. The response of the hygrometer depends on the humidity of the ambient air, and on such factors as the ventilation rate of the ambient air past the mirror, the sensitivity of the condensate detector, and the maximum cooling rate of the hygrometer. The worst case occurs during the initial dew-point reading after clearing the mirror of all condensates. The time it takes the hygrometer to reach equilibrium after clearing the mirror will vary from instrument to instrument. As an illustration of the magnitude of this time, the following are approximate times required by a hygrometer to reach equilibrium after clearing the mirror.

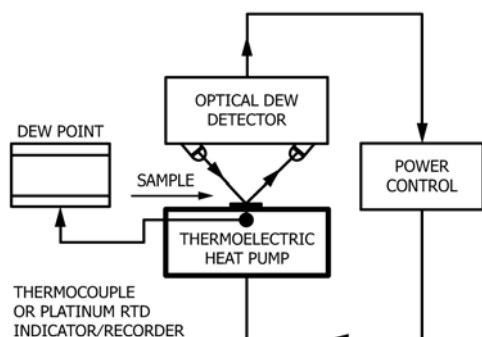


FIG. 1 Schematic of a Thermoelectric Cooled Condensation Hygrometer