



Designation: D5811 – 20

Standard Test Method for Strontium-90 in Water¹

This standard is issued under the fixed designation D5811; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers the determination of radioactive ⁹⁰Sr in environmental water samples (for example, non-process and effluent waters) in the range of 0.037 Bq/L (1.0 pCi/L) or greater.

1.2 This test method has been used successfully with tap water. It is the user's responsibility to ensure the validity of this test method for samples larger than 1 L and for waters of untested matrices.

1.3 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.* For specific hazard statements, see Section 9.

1.5 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

2.1 ASTM Standards:²

D1129 Terminology Relating to Water

D1193 Specification for Reagent Water

D1890 Test Method for Beta Particle Radioactivity of Water

D2777 Practice for Determination of Precision and Bias of Applicable Test Methods of Committee D19 on Water

D3370 Practices for Sampling Water from Flowing Process Streams

¹ This test method is under the jurisdiction of ASTM Committee D19 on Water and is the direct responsibility of Subcommittee D19.04 on Methods of Radiochemical Analysis.

Current edition approved May 1, 2020. Published June 2020. Originally approved in 1995. Last previous edition approved in 2013 as D5811 – 08 (2013). DOI: 10.1520/D5811-20.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

D3648 Practices for the Measurement of Radioactivity

D4448 Guide for Sampling Ground-Water Monitoring Wells

D5673 Test Method for Elements in Water by Inductively Coupled Plasma—Mass Spectrometry

D5847 Practice for Writing Quality Control Specifications for Standard Test Methods for Water Analysis

D6001 Guide for Direct-Push Groundwater Sampling for Environmental Site Characterization

D7282 Practice for Set-up, Calibration, and Quality Control of Instruments Used for Radioactivity Measurements

D7902 Terminology for Radiochemical Analyses

2.2 Other Documents:

ANSI N42.22 Traceability of Radioactive Sources to the National Institute of Standards and Technology (NIST) and Associated Instrument Quality Control³

BIPM-5 Decay Data Evaluation Project (DDEP)⁴

NUDAT2⁵

3. Terminology

3.1 Definitions:

3.1.1 For definitions of terms used in this standard, refer to Terminology D1129.

3.1.2 For definitions of terms used in this standard relating to radiochemical analysis, refer to Terminology D7902.

4. Summary of Test Method

4.1 This test method is based on the utilization of solid phase extraction of strontium from water samples with detection of the radioactive strontium by gross beta gas proportional counting.

4.2 An aliquant of the sample is measured into a beaker, strontium carrier added, digested with nitric acid, sorbed on an ion exchange column, eluted, evaporated to dryness, dissolved in nitric acid (8 M), selectively sorbed on a solid phase extraction column, eluted with dilute nitric acid, dried on a planchet. The sample test source (STS) is counted for beta radiation.

4.3 Fig. 1 shows a flow diagram for this test method.

³ Available from Institute of Electrical and Electronics Engineers, Inc. (IEEE), 445 Hoes Ln., Piscataway, NJ 08854-4141, <http://www.ieee.org>.

⁴ Available from BIPM, Sèvres Cedex, France, <https://www.bipm.org>.

⁵ Available from National Nuclear Data Center at Brookhaven National Laboratory, W Princeton Ave, Yaphank, NY 11980, <http://www.nndc.bnl.gov>.

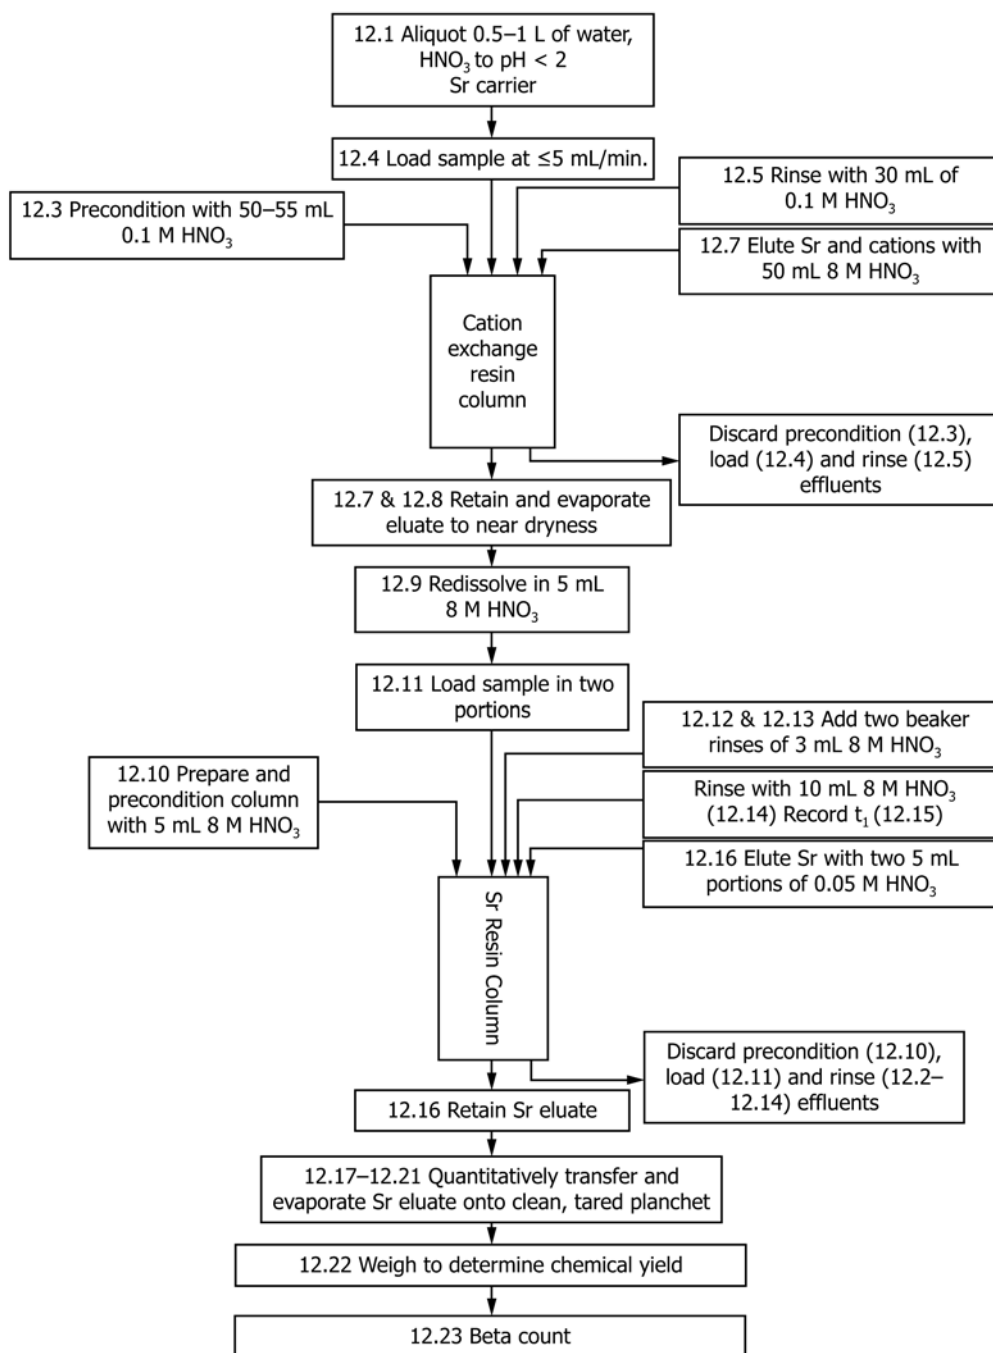


FIG. 1 Flow Diagram for the Procedure

5. Significance and Use

5.1 This test method was developed to measure the concentration of ^{90}Sr in non-process water samples. This test method may be used to determine the concentration of ^{90}Sr in environmental samples.

6. Interferences

6.1 Significant amounts of stable strontium native to the sample will interfere with the yield determination. If natural strontium is known or suspected to be present in the sample at levels that will compromise the determination of the chemical

yield, analyze sample aliquots to which no strontium carrier has been added to determine the natural strontium content. Alternatively, the elemental strontium concentration may be determined using an appropriate method such as ICP-MS, Test Method D5673. Account for the amount of natural strontium contained in the sample when calculating the chemical yield correction factor.

6.2 Strontium-89 present in the sample will cause a high bias in proportion to the $^{89}\text{Sr}/^{90}\text{Sr}$ ratio. This technique is not applicable when it is suspected or known that ^{89}Sr is present in the sample.

6.3 Strontium nitrate ($\text{Sr}(\text{NO}_3)_2$) is hygroscopic. This chemical property may add uncertainty in the gravimetric yield determination of the chemical yield.

7. Apparatus

7.1 *Analytical Balance*, 0.0001 g.

7.2 *Low Background Gas Proportional Beta Counting System*.

7.3 *Ion Exchange Columns*, 10 mL resin capacity, glass or acid-resistant plastic. An attached reservoir of at least 50 mL is desirable.

7.4 *Planchets*, stainless steel to match calibration source.⁶

8. Reagents and Materials

8.1 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to specifications of the Committee on Analytical Reagents of the American Chemical Society.⁷ Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination. Some reagents, even those of high purity, may contain naturally-occurring radioactivity, such as isotopes of uranium, radium, actinium, thorium, rare earths, potassium compounds, or artificially produced radionuclides, or combinations thereof. Consequently, when such reagents are used in the analysis of low-radioactivity samples, the activity of the reagents should be determined under analytical conditions that are as close as practicable to those used for the test sample. The activity contributed by the reagents should be accounted for and applied as a correction when calculating the test sample result.

8.2 *Purity of Water*—Unless otherwise indicated, reference to water shall be understood to mean reagent water conforming to Specification D1193, Type III.

8.3 *Cation Exchange Resin*, 100 to 200 mesh, hydrogen form. 8 % cross linked, analytical grade.

8.4 *Nitric Acid* (sp gr 1.42)—Concentrated HNO_3 .

8.5 *Nitric Acid* (8 M HNO_3)—Add 500 mL of concentrated HNO_3 to 400 mL of water. Dilute to 1 L with water.

8.6 *Nitric Acid* (0.1 M HNO_3)—Add 6.4 mL of concentrated HNO_3 to 600 mL of water. Dilute to 1 L with water.

8.7 *Nitric Acid* (0.05 M HNO_3)—Add 3.2 mL of concentrated HNO_3 to 600 mL of water. Dilute to 1 L with water.

8.8 *Strontium Carrier* (10 g/L)—Preferably use 10 000 µg/mL ICP standard. Alternatively, dissolve 24.16 g dry strontium nitrate ($\text{Sr}(\text{NO}_3)_2$) in water, add 20 mL concentrated nitric acid, and dilute with water to 1 L. Use the following

procedure to standardize the prepared strontium carrier: Carefully pipet a 5.0 mL portion of the strontium carrier solution onto a clean, dried, and tared planchet. Dry the planchet under the same conditions used for the final evaporation in 12.20. Allow the planchet to cool to room temperature and reweigh the planchet to the nearest 0.0001 g. Divide the net weight by 10. This result is the amount of strontium nitrate actually added. Use an average of three values in the denominator of the chemical yield equation in 11.12 and 13.1. This value should be within 3 % of 12.08 mg/0.5 mL.

8.9 *Strontium Extraction Chromatography Column*, 2 mL bed volume consisting of an octanol solution of 4,4'-(5')-bis (t-butyl-cyclohexano)-18-crown-6 sorbed on an inert polymeric support.⁸

8.10 *Strontium-90 Standardizing Solution*—Solution with a final concentration typically ranging from 85 to 125 Bq/mL and less than 0.1 mg of stable strontium, traceable to the SI through a national metrology institute (NMI), such as National Institute of Standards and Technology (NIST).

9. Hazards

9.1 Use extreme caution when handling all acids. They are extremely corrosive and skin contact could result in severe burns.

9.2 When diluting concentrated acids, always use safety glasses and protective clothing, and add the acid to the water.

10. Sampling

10.1 Collect a sample in accordance with Practices D3370, Guide D4448, and Guide D6001, or other documented procedure.

11. Calibration

11.1 Calibrate the low background gas proportional beta counting system in accordance with Practice D7282, Sections 14, 15, and 16. Prepare a set of three working calibration standards (WCS) according to the procedure outlined in the subsequent steps.

11.2 Pipet 0.5 mL of strontium carrier into a small beaker.

11.3 Add 1 mL of traceable ^{90}Sr solution and evaporate to near dryness on a hot plate.

11.4 Redissolve the residual in 5 mL of 8 M nitric acid.

11.5 Follow the steps described in 12.10 through 12.23.

11.6 Count to accumulate 10 000 net counts in the counting period. Counting should be completed within 3 h of column elution. Record the time and date of the midpoint of this counting period as t_2 . Count each WCS twice, once for this step having a counting date designated as t_2 and a second time as specified below.

11.7 Calculate the net count rate of the WCS at time t_2 ($R_{n(2)}$) by subtracting the instrument background count rate from the gross count rate.

⁶ Stainless steel planchets available commercially have been found satisfactory.

⁷ ACS Reagent Chemicals, Specifications and Procedures for Reagents and Standard-Grade Reference Materials, American Chemical Society, Washington, DC. For suggestions on the testing of reagents not listed by the American Chemical Society, see *Analar Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD.

⁸ Sr resin available commercially have been found satisfactory.