Designation: E2007 – 10 (Reapproved 2016)

Standard Guide for Computed Radiography[1]

This standard is issued under the fixed designation E2007; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ε) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This guide provides general tutorial information regarding the fundamental and physical principles of computed radiography (CR), definitions and terminology required to understand the basic CR process. An introduction to some of the limitations that are typically encountered during the establishment of techniques and basic image processing methods are also provided. This guide does not provide specific techniques or acceptance criteria for specific end-user inspection applications. Information presented within this guide may be useful in conjunction with those standards of 1.2.

1.2 CR techniques for general inspection applications may be found in Practice E2033. Technical qualification attributes for CR systems may be found in Practice E2445. Criteria for classification of CR system technical performance levels may be found in Practice E2446. Reference Images Standards E2422, E2660, and E2669 contain digital reference acceptance illustrations.

1.3 The values stated in SI units are to be regarded as the standard. The inch-pound units given in parentheses are for information only.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*[2]

E94 Guide for Radiographic Examination

E746 Practice for Determining Relative Image Quality Response of Industrial Radiographic Imaging Systems

E747 Practice for Design, Manufacture and Material Grouping Classification of Wire Image Quality Indicators (IQI) Used for Radiology

E1025 Practice for Design, Manufacture, and Material Grouping Classification of Hole-Type Image Quality Indicators (IQI) Used for Radiology

E1316 Terminology for Nondestructive Examinations

E1453 Guide for Storage of Magnetic Tape Media that Contains Analog or Digital Radioscopic Data

E2002 Practice for Determining Total Image Unsharpness and Basic Spatial Resolution in Radiography and Radioscopy

E2033 Practice for Computed Radiology (Photostimulable Luminescence Method)

E2339 Practice for Digital Imaging and Communication in Nondestructive Evaluation (DICONDE)

E2422 Digital Reference Images for Inspection of Aluminum Castings

E2445 Practice for Performance Evaluation and Long-Term Stability of Computed Radiography Systems

E2446 Practice for Manufacturing Characterization of Computed Radiography Systems

E2660 Digital Reference Images for Investment Steel Castings for Aerospace Applications

E2669 Digital Reference Images for Titanium Castings

2.2 *SMPTE Standard:*

RP-133 Specifications for Medical Diagnostic Imaging Test Pattern for Television Monitors and Hard-Copy Recording Cameras[3]

3. Terminology

3.1 Unless otherwise provided within this guide, terminology is in accordance with Terminology E1316.

3.2 *Definitions:*

3.2.1 *aliasing*—artifacts that appear in an image when the spatial frequency of the input is higher than the output is capable of reproducing. This will often appear as jagged or stepped sections in a line or as moiré patterns.

3.2.2 *basic spatial resolution (SR_b)*—terminology used to describe the smallest degree of visible detail within a digital image that is considered the effective pixel size.

[1] This guide is under the jurisdiction of ASTM Committee E07 on Nondestructive Testing and is the direct responsibility of Subcommittee E07.01 on Radiology (X and Gamma) Method.

Current edition approved July 1, 2016. Published July 2016. Originally approved in 1999. Last previous edition approved in 2010 as E2007 -10. DOI: 10.1520/E2007-10R16.

[2] For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

[3] Available from Society of Motion Picture and Television Engineers (SMPTE), 3 Barker Ave, 5th Floor, White Plains, NY 10601.

Copyright © ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959. United States

Documents
Document Sharing Hub
Full document details: ASTM E2007-10(2016)

3.2.2.1 *Discussion*—The concept of basic spatial resolution involves the ability to separate two distinctly different image features from being perceived as a single image feature. When two identical image features are determined minimally distinct, the single image feature is considered the effective pixel size. If the physical sizes of the two distinct features are known, for example, widths of two parallel lines or bars with an included space equal to one line or bar, then the effective pixel size is considered ½ of their sums. Example: A digital image is determined to resolve five line pairs per mm or a width of line equivalent to five distinct lines within a millimetre. The basic spatial resolution is determined as 1/ [2 × 5 LP/ mm] or 0.100 mm.

3.2.3 *binary/digital pixel data*—a matrix of binary (0's, 1's) values resultant from conversion of PSL from each latent pixel (on the IP) to proportional (within the bit depth scanned) electrical values. Binary digital data value is proportional to the radiation dose received by each pixel.

3.2.4 *bit depth*—the number "2" increased by the exponential power of the analogue-to-digital (A/D) converter resolution. Example *1*) In a 2-bit image, there are four (2^2) possible combinations for a pixel: 00, 01, 10 and 11. If "00" represents black and "11" represents white, then "01" equals dark gray and "10" equals light gray. The bit depth is two, but the number of gray scales shades that can be represented is 2^2 or 4. Example *2*): A 12-bit A/D converter would have 4096 (2^{12}) gray scales shades that can be represented.

3.2.5 *blooming or flare*—an undesirable condition exhibited by some image conversion devices brought about by exceeding the allowable input brightness for the device, causing the image to go into saturation, producing an image of degraded spatial resolution and gray scale rendition.

3.2.6 *computed radiographic system*—all hardware and software components necessary to produce a computed radiograph. Essential components of a CR system consisting of: an imaging plate, an imaging plate readout scanner, electronic image display, image storage and retrieval system and interactive support software.

3.2.7 *computed radiographic system class*—a group of computed radiographic systems characterized with a standard image quality rating. Practice E2446, Table 1, provides such a classification system.

3.2.8 *computed radiography*—a radiological nondestructive testing method that uses storage phosphor imaging plates (IP's), a PSL stimulating light source, PSL capturing optics, optical-to-electrical conversion devices, analogue-to-digital data conversion electronics, a computer and software capable of processing original digital image data and a means for electronically displaying or printing resultant image data.

3.2.9 *contrast and brightness*—an application of digital image processing used to "re-map" *displayed* gray scale levels of an *original* gray scale data matrix using different reference lookup tables.

3.2.9.1 *Discussion*—This mode of image processing is also known as "windowing" (contrast adjustment) and "leveling" (brightness adjustment) or simply "win-level" image processing.

3.2.10 *contrast-to-noise ratio (CNR)*—quotient of the digital image contrast (see 3.2.13) and the averaged standard deviation of the linear pixel values.

3.2.10.1 *Discussion*—CNR is a measure of image quality that is dependent upon both digital image contrast and signal-to-noise ratio (SNR) components. In addition to CNR, a digital radiograph must also possess adequate sharpness or basic spatial resolution to adequately detect desired features.

3.2.11 *digital driving level (DDL)*—terminology used to describe displayed pixel brightness of a digital image on a monitor resultant from digital mapping of various gray scale levels within specific look-up-table(s).

3.2.11.1 *Discussion*— DDL is also known as monitor pixel intensity value; thus, may not be the PV of the original digital image.

3.2.12 *digital dynamic range*—maximum material thickness latitude that renders acceptable levels of specified image quality performance within a specified pixel intensity value range.

3.2.12.1 *Discussion*—Digital dynamic range should not be confused with computer file bit depth.

3.2.13 *digital image contrast*—pixel value difference between any two areas of interest within a computed radiograph.

3.2.13.1 *Discussion*—digital contrast = **PV2 – PV1** where PV2 is the pixel value of area of interest "2" and PV1 is the pixel value of area of interest "1" on a computed radiograph. Visually displayed image contrast can be altered via digital re-mapping (see 3.2.11) or re-assignment of specific gray scale shades to image pixels.

3.2.14 *digital image noise*—imaging information within a computed radiograph that is not directly correlated with the degree of radiation attenuation by the object or feature being examined and/or insufficient radiation quanta absorbed within the detector IP.

3.2.14.1 *Discussion*—Digital image noise results from random spatial distribution of photons absorbed within the IP and interferes with the visibility of small or faint detail due to statistical variations of pixel intensity value.

3.2.15 *digital image processing*—the use of algorithms to change original digital image data for the purpose of enhancement of some aspect of the image.

3.2.15.1 *Discussion*—Examples include: contrast, brightness, pixel density change (digital enlargement), digital filters, gamma correction and pseudo colors. Some digital processing operations such as sharpening filters, once saved, permanently change the original binary data matrix (Fig. 1, Step 5).

3.2.16 *equivalent penetrameter sensitivity (EPS)*—that thickness of penetrameter, expressed as a percentage of the section thickness radiographed, in which a 2T hole would be visible under the same radiographic conditions. EPS is calculated by: EPS% = 100/ X (√ Th/2), where: h = hole diameter, T = step thickness and X= thickness of test object (see E1316, E1025, E747, and Practice E746).

3.2.17 *gray scale*—a term used to describe an image containing shades of gray rather than color. Gray scales are used

AVA Documents
Document Sharing Hub

Full document details: ASTM E2007-10(2016)

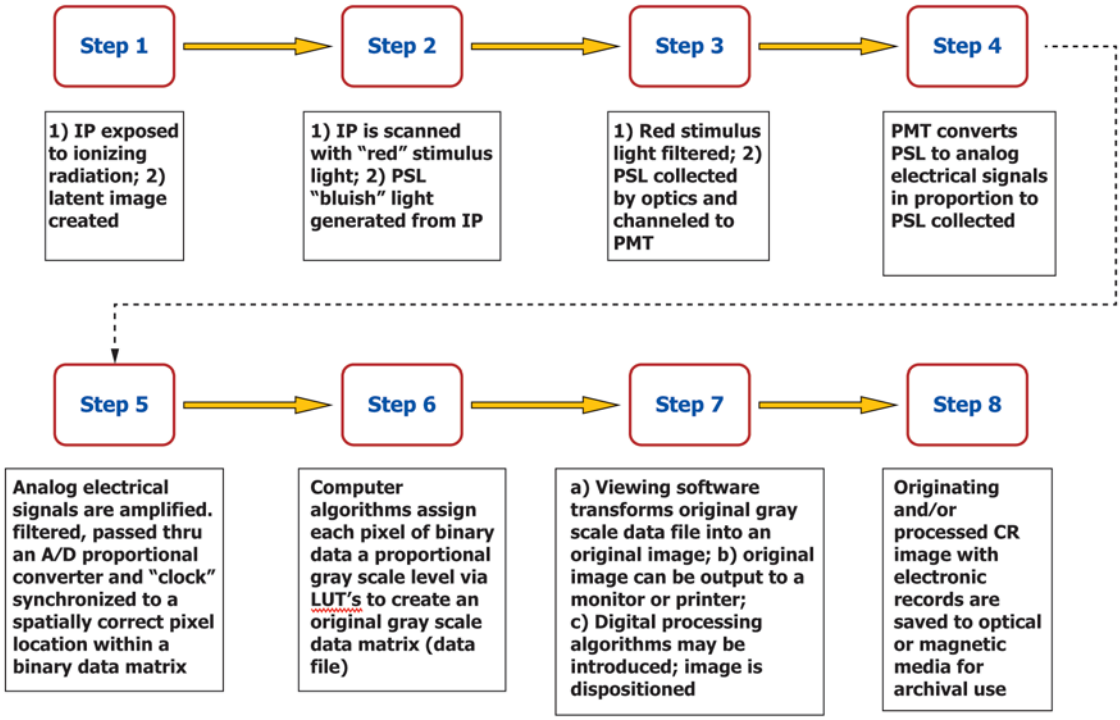

FIG. 1 Basic Computed Radiography Process

of gray shades assigned to image pixels that result in visually perceived pixel display brightness.

3.2.17.1 *Discussion*—The number of shades is usually positive integer values taken from the bit depth. For example: an 8-bit gray scale image has up to 256 total shades of gray from 0 to 255, with 0 representing white image areas and 255 representing black image areas with 254 shades of gray in between.

3.2.18 *image morphing*—a potentially degraded CR image resultant from over processing (that is, over driving) an original CR image.

3.2.18.1 *Discussion*—"Morphing" can occur following several increments of image processing where each preceding image was "overwritten" resulting in an image that is noticeably altered from the original.

3.2.19 *look up table (LUT)*—one or more fields of binary digital values arbitrarily assigned to a range of reference gray scale levels (viewed on an electronic display as shades of "gray").

3.2.19.1 *Discussion*—A LUT is used (applied) to convert binary digital pixel data to proportional shades of "gray" that define the CR image. LUT's are key reference files that allow binary digital pixel data to be viewed with many combinations of pixel gray scales over the entire range of a digital image (see Fig. 5-A).

3.2.20 *original digital image*—a digital gray scale (see 3.2.17) image resultant from application of original binary digital pixel data to a linear look-up table (see 3.2.24 and 3.2.19 prior to any image processing.

3.2.20.1 *Discussion*—This original gray scale image is usually considered the beginning of the "computed radiograph", since without this basic conversion (to gray scales) there would be no discernable radiographic image (see Fig. 5-B).

3.2.21 *photostimulable luminescence (PSL)*—photostimulable luminescence (PSL) is a physical phenomenon in which a halogenated phosphor compound emits bluish light when excited by a source of red spectrum light.

3.2.22 *pixel brightness*—the luminous (monitor) display intensity of pixel(s) that can be controlled by means of electronic monitor brightness level settings or changes of digital driving level (see 3.2.11).

3.2.23 *pixel density*—the number of pixels within a digital image of fixed dimensions (that is, length and width).

3.2.23.1 *Discussion*—for digital raster images, the convention is to describe pixel density in terms of the number of pixel-columns (width) and number of pixel rows (height). An alternate convention is to describe the total number of pixels in the image area (typically given as the number of mega pixels), which can be calculated by multiplying pixel-columns by pixel-rows. Another convention includes describing pixel density per area-unit or per length-unit such as pixels per in./mm. Resolution (see 7.1.5) of a digital image is related to pixel density.

3.2.24 *pixel value (PV)*—a positive integer numerical value directly associated with each binary picture data element (pixel) of an original digital image where gray scale shades (see 3.2.17) are assigned in linear proportion to radiation exposure dose received by that area.

3.2.24.1 *Discussion*—Computed radiography uses gray scale shades to render visual perceptions of image contrast; thus, linear pixel value (PV) is used to measure a specific shade

AVA Documents
Document Sharing Hub

Full document details: ASTM E2007-10(2016)

of gray that corresponds to the quantity of radiation exposure absorbed within a particular area of a part. With this relationship, a PV of "0" can correspond with "0" radiation dose (white image area of a negative image view) whereas a PV of "4095" can correspond with a saturated detector (black image area of a negative image view) for a 12 bit CR system. PV is directly related to original binary pixel data via a common linear look-up-table (Fig. 5 A and B illustrate). The number of available pixel value integers within an image is associated with the number of available gray scale shades for the bit depth of the image.

3.2.25 *PSL afterglow*—continued luminescence from a storage phosphor immediately following removal of an external photostimulating source.

3.2.25.1 *Discussion*—A bluish luminescence continues for a short period of time after termination of the photostimulating source as illustrated in Fig. 12.

3.2.26 *relative image quality response (RIQR)*—a means for determining the image quality performance response of a given radiological imaging system in relative comparison to the image quality response of another radiological imaging system.

3.2.26.1 *Discussion*—RIQR methods are not intended as a direct measure of image quality for a specific radiographic technique application. Practice E746 provides a standard RIQR method.

3.2.27 *signal-to-noise ratio (SNR)*—quotient of mean linear pixel value and standard deviation of mean linear pixel values (noise) for a defined detector area-of-interest in a digital image.

3.2.27.1 *Discussion*—Notwithstanding extraneous sources of digital image noise, SNR will normally increase as exposure dose is increased.

3.2.28 *spatial resolution*—terminology used to define a component of optical image quality associated with distinction of closely spaced adjacent multiple features.

3.2.28.1 *Discussion*—The concept of optical resolution involves the ability to separate multiple closely spaced components, for example, optical line pairs, into two or more distinctly different components within a defined unit of space. Example: an optical imaging system that is said to resolve two line pairs within one mm of linear space (that is, 2 Lp/mm) contains five individual components: two closely spaced adjacent line components, an intervening space between the lines and space on the outside boundaries of the two lines.

3.2.29 *storage phosphor imaging plate (IP)*—a photostimulable luminescent material that is capable of storing a latent radiographic image of a material being examined and, upon stimulation by a source of red spectrum light, will generate luminescence (PSL) proportional to radiation absorbed.

3.2.29.1 *Discussion*—When performing computed radiography, an IP is used in lieu of a film. When establishing techniques related to source focal geometries, the IP is referred to as a detector (i.e. source-to detector-distance or SDD).

3.2.30 *unsharpness*—terminology used to describe an attribute of image quality associated with blurring or loss of distinction within a radiographic image.

3.2.30.1 *Discussion*—Measured total unsharpness is described with a numerical value corresponding with a measure of definition (that is, distinction) associated with the geometry of exposure and inherent unsharpness of the CR system (that is, inherent or total unsharpness). Guide E94 provides fundamental guidance related to geometrical unsharpness and Practice E2002 provides a standard practice for measurement of total unsharpness.

4. Significance and Use

4.1 This guide is intended as a source of tutorial and reference information that can be used during establishment of computed radiography techniques and procedures by qualified CR personnel for specific applications. All materials presented within this guide may not be suited for all levels of computed radiographic personnel.

4.2 This guide is intended to build upon an established basic knowledge of radiographic fundamentals (that is, film systems) as may be found in Guide E94. Similarly, materials presented within this guide are not intended as "all-inclusive" but are intended to address basic CR topics and issues that complement a general knowledge of computed radiography as described in 1.2 and 3.2.28.

4.3 Materials presented within this guide may be useful in the development of end-user training programs designed by qualified CR personnel or activities that perform similar functions. Computed radiography is considered a rapidly advancing inspection technology that will require the user maintain knowledge of the latest CR apparatus and technique innovations. Section 11 of this guide contains technical reference materials that may be useful in further advancement of knowledge associated with computed radiography.

5. Computed Radiography Fundamentals

5.1 This section introduces and describes primary core components and processes of a basic computed radiography process. The user of this standard guide is advised that computed radiography is a rapidly evolving technology where innovations involving core steps and processes are continually under refinement. Tutorial information presented in this section is intended to illustrate the fundamental computed radiography process and not necessarily any specific commercial CR system.

5.2 *Acquiring the CR Image:* Computed radiography (CR) is one of several different modes of digital radiography that employs re-usable photostimulable luminescence (PSL) storage phosphor imaging plates (commonly called IP's) for acquisition of radiographic images. Figure 1 illustrates an example of the fundamental steps of a basic CR process arrangement.

In this illustration, a conventional (that is, Guide E94) radiographic exposure geometry/arrangement is used to expose a part positioned between the radiation source and IP. *Step 1* involves exposure of the IP (Fig. 2 illustrates typical cross section details of an IP) and creation of a residual latent image with delayed luminescence properties (Section 6 details physics).

Step 2 involves index scanning the exposed IP with a stimulus source of red light from a laser beam (Fig. 3 illustrates Steps 2 through 8).

AVA Documents
Document Sharing Hub

Full document details: ASTM E2007-10(2016)

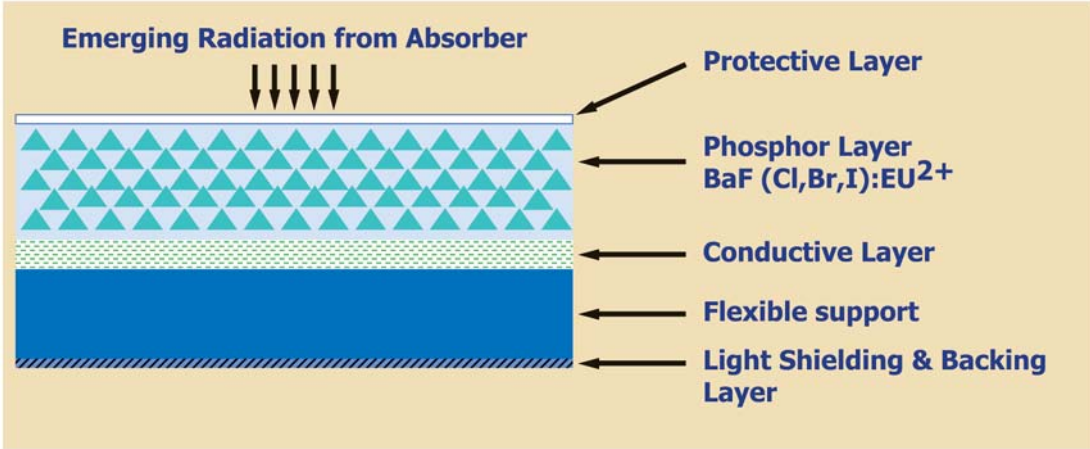

Illustration courtesy of Fujifilm NDT Systems

FIG. 2 Cross Section of a Typical Storage Phosphor Imaging Plate

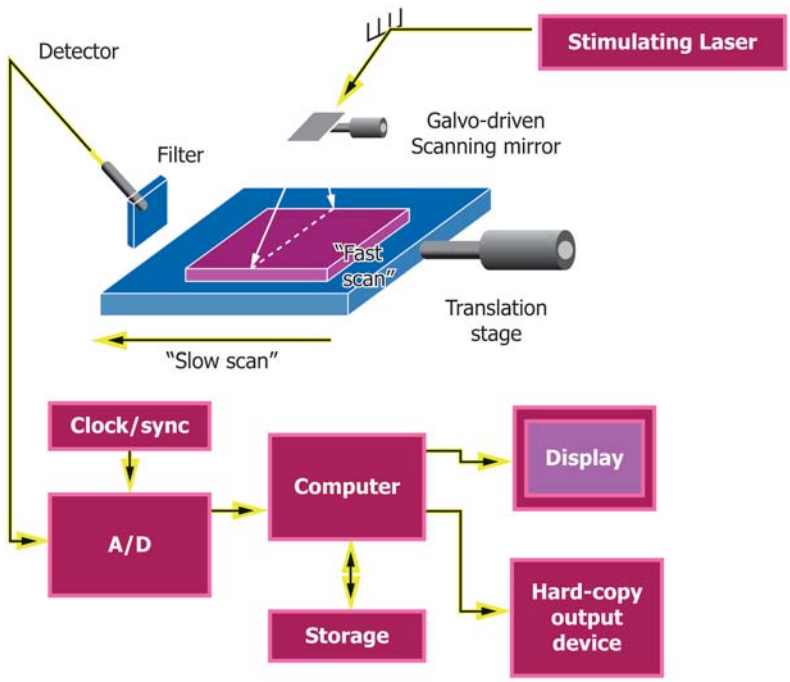

Illustration courtesy of Carestream Health

FIG. 3 Fundamental CR Image Acquisition and Display Process

During the scan, the IP is stimulated to release deposited energy of the latent image in the form of bluish photostimulated visible light. *Step 3:*the bluish photostimulated light (PSL) is then collected by an optical system containing a chromatic filter (that prevents the red stimulus light from being collected) and channeled to a photo-multiplier tube (PMT). *Step 4:*PSL light is converted by the PMT to analogue electrical signals in proportion to quantity of PSL collected. *Step 5:*analog electrical signals are amplified, filtered, passed through an analog-to-digital (A/D) converter and "clock" synchronized to a spatially correct pixel location within a binary data matrix (Fig. 4 illustrates assignment of binary data to a pixel matrix).

The actual size of the binary pixel element (length and width) is determined by the scanning speed of the transport mechanism in one direction and the clock speed of the sampling along each scan line (how fast the laser spot moves divided by the sampling rate). Although resolution is limited by pixel size, the size of individual phosphor crystals, the phosphor layer thickness of the image plate, laser spot size and optics also contribute to the overall quality (resolution) of the image. Each of these components thus becomes a very essential contributor to the overall binary matrix that represents the digital image. These individual elements represent the smallest unit of storage of a binary digital image that can be discretely controlled by the CR data acquisition and display system components and are commonly called "pixels." The term "pixel" is thus derived from two word components of the digital matrix, that is, picture (or pix) and elements (els) or "pixels." Picture elements or pixels become the basic for all

AVA Documents
Document Sharing Hub

Full document details: ASTM E2007-10(2016)

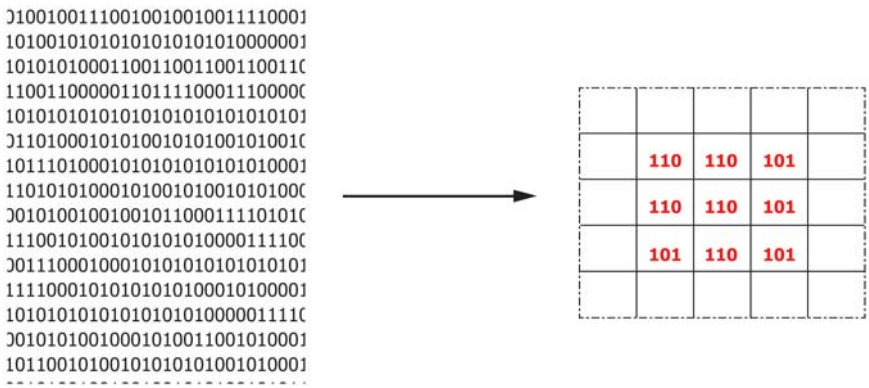

FIG. 4 Assignment of Binary Data to a Pixel Matrix (3-bit depth illustrated)

technical imaging attributes that comprise quality and composition of the resultant image. An organized matrix of picture elements (pixels) containing binary data is called a binary pixel data matrix since proportional gray levels have not yet been assigned. (see 11.1.2) contains basic tutorial information on binary numbering system and its usefulness for digital applications).

Step 6: Computer algorithms (a string of mathematical instructions) are applied that match binary pixel data with arbitrary files (called look-up-tables) to assign individual pixel gray scale levels. Example: for 4096 possible shades or levels of gray for a 12-bit image, gray scale levels are thus derived when a computer assigns equal divisions between white ("0") and black ("4095") with each incremental division a derivative (shade) of black or white (that is, gray) for a negative view image. An example is to assign gray scale levels in linear proportion to the magnitude of the binary numbers (that is, a higher binary number associated with a greater amount of photo stimulated light for that pixel registration can be assigned a corresponding darker gray value) to create an original gray scale data matrix with a standard format (DICONDE, TIFF, BITMAP, etc.) ready for software transformation. Fig. 5-A illustrates a simple linear look-up-table for an original gray scale data matrix where binary numbers are also represented by their corresponding numerical integers (called pixel value integers). In this example for a 12-bit image, there are 4096 gray scale divisions that precisely correspond with 4096 numerical pixel value integers. Fig. 5-B illustrates a graphical version of the application as might be applied by an algorithm to produce an image with a gray tonal appearance (visually similar to a radiographic film). Most algorithms employed for *original* CR images assign gray scale values in *linear* proportion to the magnitude of each binary pixel (value). The range (number) of selectable gray values is defined within the image viewing software as "bit depth."

Step 7: a) Viewing software is used to transform the original gray scale data matrix into an original image; *b*) The original image can be output to an electronic display monitor or printer; the resultant CR digital image can have a similar gray tonal appearance as its film counterpart (as illustrated with the LUT shown in Fig. 5-A in that as gray values become larger, displayed luminance becomes smaller. With the digital image display, inspected features can be characterized and dispositioned similar to a radiographic film. Both image modalities require evaluations within environments of subdued background lighting. Aside from these basic similarities, however, the CR digital image is an entirely different imaging modality that requires some basic knowledge of digital imaging fundamentals in order to understand and effectively apply the technology; *c*) Once the original digital image is visualized, additional image processing techniques (see Section 8) may be performed to further enhance inspection feature details and complete the inspection evaluation process. This entire process is called *computed* radiography because of the extreme dependence on complex computational processes in order to render a meaningful radiographic image. Finally (*Step 8*), original and/or processed digital images and related electronic records may be saved to optical, magnetic or print media for future use. Some applications may benefit from a high quality digital print of the saved image. Typical CR system commercial hardware components are illustrated in Fig. 6. Computed radiographic technology is complex in nature; therefore, subsequent sections of this standard are intended to provide some additional levels of detail associated with the *basic* computed radiography process. Additional levels of information may be found within the bibliography, Section 11.

6. Brief History and Physics of Computed Radiography

6.1 *Photo-Stimulated Luminescence (PSL)* is a physical phenomenon in which a halogenated phosphor compound emits bluish light when excited by a source of red spectrum light. In other words, phosphors capable of "PSL" exhibit a unique physical property of delayed release of visible light subsequent to radiation exposure; thus, the reason this type of phosphor is sometimes referred to as a "storage phosphor." illustrates the photo excitation process when this phosphor is exposed (following exposure of the phosphor to radiation) to a source of red light (He-Ne or semiconductor laser). The "bluish-purple" light emitted during this stimulation is referred to as "photostimulated luminescence" or "PSL" for short. During collection of PSL light for computed radiography, the red light source is **separated** from PSL using a chromatic filter (see Fig. 3). The "PSL" process is the very heart of CR technology and is thus important for understanding how computed radiography works.

AVA Documents
Document Sharing Hub

Full document details: ASTM E2007-10(2016)

12 Bit Binary Pixel Data (fig. 1, step 5)	Original LUT (fig. 1, step 6) Pixel Value Integer
0	0
1	1
10	2
11	3
100	4
101	5
↓	↓
111111111111	4095
4096 Increments of binary data	4096 Increments of gray scales

A

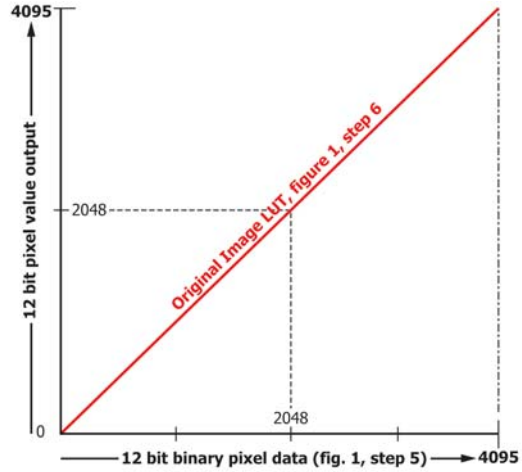

B

FIG. 5 (A) Original 12-bit Linear Look-Up Table / (B) Graph Version of Applied Linear LUT

Illustrations courtesy of Carestream Health & Fujifilm NDT Systems

FIG. 6 Typical CR Scanner, Workstation, and Image Plate

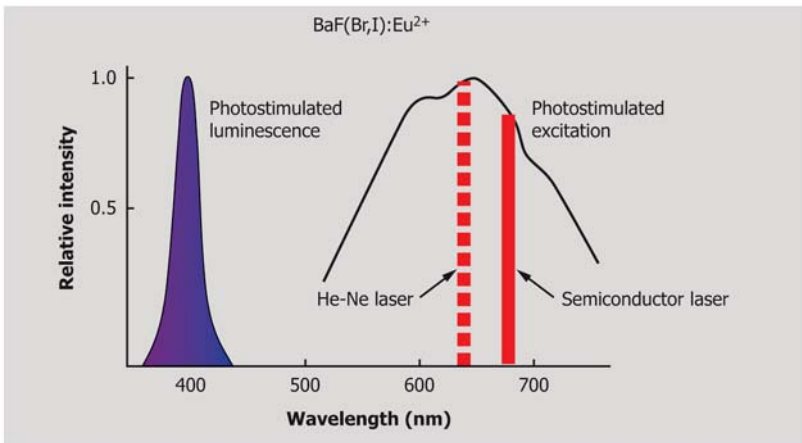

Illustration courtesy of Fujifilm NDT Systems

FIG. 7 Spectra of Photostimulated Luminescence and Excitation

6.2 *Early History of Photo Stimulated Luminensce:* The earliest written reference to fluorescence, the phenomenon that causes materials to emit light in response to external stimuli, dates back to 1500 B.C. in China. This phenomenon did not attract scientific interest until 1603, when the discovery of the Bolognese stone in Italy led to investigation by a large number

AVA Documents
Document Sharing Hub

Full document details: ASTM E2007-10(2016)