



Designation: E422 – 22

Standard Test Method for Measuring Net Heat Flux Using a Water-Cooled Calorimeter¹

This standard is issued under the fixed designation E422; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers the measurement of a steady net heat flux to a given water-cooled surface by means of a system energy balance.

1.2 *Units*—The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.*

1.4 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

2.1 ASTM Standards:²

E176 Terminology of Fire Standards

E230/E230M Specification for Temperature-Electromotive Force (emf) Tables for Standardized Thermocouples

E235 Specification for Type K and Type N Mineral-Insulated, Metal-Sheathed Thermocouples for Nuclear or for Other High-Reliability Applications

E456 Terminology Relating to Quality and Statistics

E459 Test Method for Measuring Heat Transfer Rate Using a Thin-Skin Calorimeter

E3057 Test Method for Measuring Heat Flux Using Directional Flame Thermometers with Advanced Data Analysis Techniques

¹ This test method is under the jurisdiction of ASTM Committee E21 on Space Simulation and Applications of Space Technology and is the direct responsibility of Subcommittee E21.08 on Thermal Protection.

Current edition approved April 1, 2022. Published May 2022. Originally approved in 1971. Last previous edition approved in 2016 as E422 – 05(2016). DOI: 10.1520/E0422-22.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

3. Terminology

3.1 *Definitions*—Refer to Terminologies E176 and E456 for definitions of terms used in this test method.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *absorbed heat flux, n*—incident radiative heat flux less the reflected radiative flux, W/m^2 .

3.2.2 *convective heat flux, n*—the addition or loss of energy per unit area into the sensing surface due to convection, $= h \cdot (T_{fs} - T_s)$, W/m^2 .

3.2.3 *control volume, n*—user defined volume over which an energy balance is determined.

3.2.4 *emitted heat flux, n*—energy per unit area emitted from a hot surface $-\epsilon \cdot \sigma \cdot T^4$, W/m^2 .

3.2.5 *incident radiative heat flux (irradiance; $q_{inc,r}$)*, *n*—radiative heat flux (energy per unit area) impinging on the surface of the calorimeter from an external environment, W/m^2 .

3.2.6 *heat flux or energy flux, n*—energy per unit area, W/m^2 .

3.2.7 *net heat flux or net energy flux, n*—net energy divided by the sensing surface area transferred to the calorimeter face; it is equal to the [absorbed radiative heat flux + convective heat flux] – [re-radiation from the exposed surface].

3.2.8 *reflected heat flux, n*—that part of the incident radiative flux that is not absorbed by or transmitted into the surface of the calorimeter, W/m^2 .

3.2.9 *verified, n*—the process of checking that a data acquisition channel correctly measures an input value, to a pre-set, acceptable level condition defined by the user.

3.3 Symbols:

A—sensing surface area of calorimeter, m^2

C_p—water specific heat, $\text{J/(kg} \cdot \text{K)}$

h—convective heat transfer coefficient, $\text{W/m}^2 \cdot \text{K}$

m—mass flow rate of coolant water, kg/sec

q—heat flux, W/m^2

T—temperature, K

T₀₁—calorimeter water inlet bulk temperature during operation, K

T₀₂—calorimeter water exhaust bulk temperature during operation, K

T_I —calorimeter water inlet bulk temperature before operation, K

T_2 —calorimeter water exhaust bulk temperature before operation, K

$\Delta T_0 = T_{02} - T_{01}$ —calorimeter water bulk temperature rise during operation, K

$\Delta T_1 = T_2 - T_1$ —calorimeter water apparent bulk temperature rise before operation, K

ϵ —emissivity of sensing surface

σ —Stefan-Boltzmann constant, $5.67\text{E-}08 \text{ W/m}^2\cdot\text{K}^4$

3.4 Abbreviations:

3.4.1 TC—thermocouple

3.4.2 PPE—personal protective equipment

3.4.3 U_{95} —total uncertainty to 95 % confidence

3.4.4 t_{95} —“Students t”

3.4.5 B_T —total bias uncertainty

3.4.6 S_T —total systematic or precision uncertainty

3.4.7 DOF—degrees of freedom

4. Summary of Test Method

4.1 A measure of the net heat flux to a given water-cooled surface is based upon the following measurements: (1) the water mass flow rate and (2) the temperature rise of coolant water. The net heat flux is determined numerically by multiplying the water coolant flow rate by the specific heat and rise in temperature of the water and dividing this value by the surface area across which heat has been transferred.

4.2 The apparatus for measuring net heat flux by the energy-balance technique is illustrated schematically in Fig. 1. It is a typical constant-flow water calorimeter used to measure stagnation region net heat flux to a flat-faced specimen. Other calorimeter shapes can also be easily used. The net heat flux is measured using the central circular sensing area, shown in Fig. 1. The water-cooled annular guard ring serves the purpose of preventing heat transfer to the sides of the calorimeter and establishes flat-plate flow. An energy balance on the control volume that surrounds the sensing surface (the centrally located calorimeter in Fig. 1) requires that the energy crossing the sensing surface (A , in Fig. 1) of the calorimeter be equated to the energy absorbed by the calorimeter cooling water.

Interpretation of the data obtained is not within the scope of this discussion; consequently, such effects as recombination efficiency of the surface and thermochemical state of the boundary layer are outside the scope of this test method. It should be noted that recombination effects at low pressures can cause serious discrepancies in net heat flux measurements (such as discussed in Ref (1))³ depending upon the surface material on the calorimeter.

4.3 For the particular control volume cited, the energy balance can be written as follows:

$$E_{\text{CAL}} = [mC_p(\Delta T_0 - \Delta T_1)]/A \quad (1)$$

where:

E_{CAL} = energy flux (or net heat flux) transferred to calorimeter face, $\text{W}\cdot\text{m}^{-2}$,

m = mass flow rate of coolant water, $\text{kg}\cdot\text{s}^{-1}$,

C_p = water specific heat, $\text{J}\cdot\text{kg}^{-1}\cdot\text{K}^{-1}$,

$\Delta T_0 = T_{02} - T_{01}$, calorimeter water bulk temperature rise during operation, K,

$\Delta T_1 = T_2 - T_1$, calorimeter water apparent bulk temperature rise before operation, K,

T_{02} = calorimeter water exhaust bulk temperature during operation, K,

T_{01} = calorimeter water inlet bulk temperature during operation, K,

T_2 = calorimeter water exhaust bulk temperature before operation, K,

T_1 = calorimeter water inlet bulk temperature before operation, K, and

A = sensing surface area of calorimeter, m^2 .

4.4 An examination of Eq 1 shows that to obtain a value of the energy transferred to the calorimeter, measurements must be made of the water coolant flow rate, the temperature rise of the coolant, and the surface area across which heat is transferred. With regard to the latter quantity, it is assumed that the surface area to which heat is transferred is well defined. As is indicated in Fig. 1, the design of the calorimeter is such that the heat transfer area is confined by design to the front or directly heated surface. To minimize side heating or side heat losses, a

³ The boldface numbers in parentheses refer to the list of references at the end of this test method.

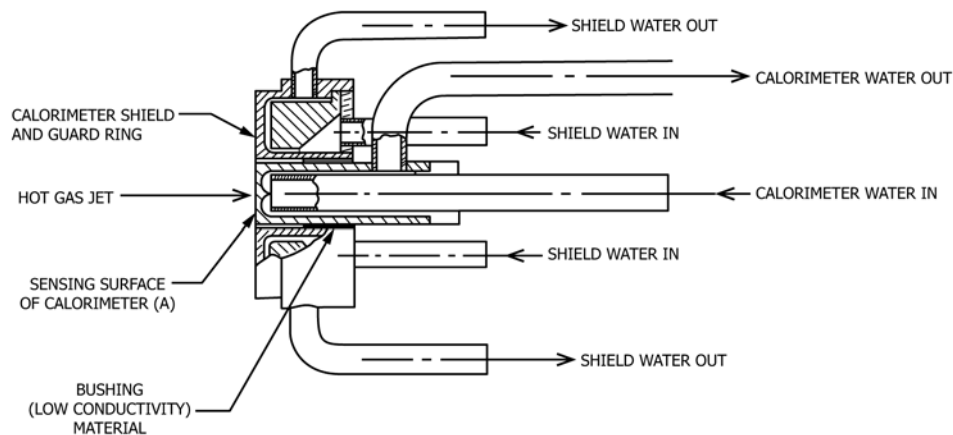


FIG. 1 Steady-State Water-Cooled Calorimeter.

water-cooled guard ring or shroud is utilized and is separated physically from the calorimeter by means of an air gap and low conductivity bushing such as nylon. The air gap is recommended to be no more than 0.5 mm on the radius. Thus, if severe pressure variations exist across the face of the calorimeter, side heating caused by flow into and out of the air gap will be minimized. Also, since the water-cooled calorimeter and guard ring operate at low surface temperatures (usually lower than 100 °C) heat losses across the gap by radiant interchange are negligible and consequently no special calorimeter surface gap finishes are necessary. Depending upon the size of the calorimeter surface, large variations in net heat flux may exist across the face of the calorimeter. Consequently, the measured net heat flux represents an average net heat flux over the surface area of the water-cooled calorimeter. The water-cooled calorimeter can be used to measure net heat flux levels over a range from 10 kW/m² to 60 MW/m².

5. Significance and Use

5.1 The purpose of this test method is to measure the net heat flux to a water-cooled surface for purposes of calibration of the thermal environment into which test specimens are placed for evaluation. The measured net heat flux is one of the important parameters for correlating the behavior of materials. If the calorimeter and holder size, shape, and surface finish are identical to that of the test specimen, the measured net heat flux to the calorimeter is presumed to be the same as that to the sample's heated surface. If the calorimeter configuration (holder size, shape, finish, etc.) is not identical to that of the test specimen, then the measurement results may need to be modified to account for those differences. See [Appendix X1](#).

5.2 The water-cooled calorimeter is one of several calorimeter concepts used to measure net heat flux. The prime drawback is its long response time, that is, the time required to achieve steady-state operation. To calculate energy added to the coolant water, accurate measurements of the rise in coolant temperature are needed, all energy losses should be minimized, and steady-state conditions must exist both in the thermal environment and fluid flow of the calorimeter.

5.3 Regardless of the source of energy input to the water-cooled calorimeter surface (radiative, convective, or combinations thereof) the measurement is averaged over the surface-active area of the calorimeter. If the water-cooled calorimeter is used to measure only radiative flux or combined convective-radiative net heat flux rates, then the surface reflectivity of the calorimeter shall be measured over the wavelength region of interest (depending on the source of radiant energy). If non-uniformities exist in the gas stream, a large surface area water-cooled calorimeter would tend to smooth or average any variations. Consequently, it is advisable that the size of the calorimeter be limited to relatively small surface areas and applied to where the net heat flux is uniform. Where large samples are tested, it is recommended that a number of smaller diameter water-cooled calorimeters be used (rather than one large unit). These shall be located across the heated surface such that a net heat flux distribution can be described. With

this, a more detailed net heat flux measurement can be applied to the specimen test and more information can be deduced from the test.

6. Apparatus

6.1 *General*—The apparatus shall consist of a water-cooled calorimeter and the necessary instrumentation to measure the heat transferred to the calorimeter. Although the recommended instrumentation accuracies are state-of-the-art values, more rugged and higher accuracy instrumentation may be required for high pressure and high net heat applications. A number of materials can be used to fabricate the calorimeter, but oxygen free high conductivity (OFHC) copper is often preferred because of its superior thermal properties. The user should decide before fabrication and use of the water-cooled calorimeter what the total acceptable uncertainty is for the application of interest. Some applications can accommodate larger uncertainties than others, and typically the smaller the required uncertainty, the higher the cost. For the water-cooled calorimeter, there are four parameters that can be uncertain: the water flow rate, the temperature difference, the water specific heat, and the sensing surface area. The acceptable total uncertainty should be expressed as xx % of reading or maximum value good to a certain confidence level. An example (but not a recommended value) would be a ± 5 % uncertainty to 95 % confidence level.

6.2 *Coolant Flow Measurement*—The water flow rate to each component of the calorimeter shall be chosen to cool the apparatus adequately and to ensure accurately measurable rise in water temperature. The error in water flow rate measurement should be not more than ± 2 %, assuming this value has been apportioned with the total acceptable uncertainty preferred. Suitable equipment that can be used is listed in Refs (2, 3) and includes turbine flowmeters, variable area flowmeters, etc. Care must be exercised in the use of all these devices. In particular, it is recommended that appropriate filters be placed in all water inlet lines to prevent particles or unnecessary deposits from being carried to the water-cooling passages, pipe, and meter walls. Water flow rates and pressure shall be adjusted to ensure that no bubbles are formed (no boiling). If practical, the water flowmeters shall be placed upstream of the calorimeter in straight portions of the piping. The flowmeter device shall be checked and calibrated periodically. Pressure gages, if required, shall be used in accordance with the manufacturer's instructions and calibration charts.

6.3 *Coolant Temperature Measurement*—The method of temperature measurement must be sufficiently sensitive and reliable to ensure accurate measurement of the coolant water temperature rise. There are two calorimeter water temperature sensors in the calorimeter, one to measure inlet water temperature and the other to measure outlet water temperature. Procedures similar to those given in Specification E235, Type K (chromel/alumel, range 0 °C to 1260 °C, accuracy ± 2.2 °C or 0.75 % of reading in °C, whichever is greater, for standard tolerances), and Ref (4) should be followed in the calibration and preparation of temperature sensors. Specification E230/E230M provides information on thermocouples (TCs) with a smaller temperature range and higher accuracy than type K