



BSI Standards Publication

Safety requirements for electrical equipment for measurement, control and laboratory use

Part 2-012: Particular requirements for climatic and environmental
testing and other temperature conditioning equipment

National foreword

This British Standard is the UK implementation of EN IEC 61010-2-012:2022+A11:2022. It is derived from IEC 61010-2-012:2019. It supersedes BS EN 61010-2-012:2016, which will be withdrawn on 29 April 2025.

The start and finish of text introduced or altered by amendment A11 is indicated in the text by tags. Tags indicating changes to text carry the number of the CENELEC amendment. For example, text altered by CENELEC amendment A11 is indicated by A11 A11.

The UK participation in its preparation was entrusted to Technical Committee EPL/66, Safety of measuring, control and laboratory equipment.

A list of organizations represented on this committee can be obtained on request to its committee manager.

Contractual and legal considerations

This publication has been prepared in good faith, however no representation, warranty, assurance or undertaking (express or implied) is or will be made, and no responsibility or liability is or will be accepted by BSI in relation to the adequacy, accuracy, completeness or reasonableness of this publication. All and any such responsibility and liability is expressly disclaimed to the full extent permitted by the law.

This publication is provided as is, and is to be used at the recipient's own risk.

The recipient is advised to consider seeking professional guidance with respect to its use of this publication.

This publication is not intended to constitute a contract. Users are responsible for its correct application.

© The British Standards Institution 2022
Published by BSI Standards Limited 2022

ISBN 978 0 580 52308 3

ICS 19.080

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 October 2022.

Amendments/corrigenda issued since publication

Date	Text affected
<hr/>	

English Version

Safety requirements for electrical equipment for measurement,
control and laboratory use - Part 2-012: Particular requirements
for climatic and environmental testing and other temperature
conditioning equipment
(IEC 61010-2-012:2019)

Règles de sécurité pour appareils électriques de mesurage,
de régulation et de laboratoire - Partie 2-012: Exigences
particulières pour les appareils d'essais climatiques et
d'environnement, et autres appareils de conditionnement de
température
(IEC 61010-2-012:2019)

Sicherheitsbestimmungen für elektrische Mess-, Steuer-,
Regel- und Laborgeräte - Teil 2-012: Besondere
Anforderungen an Klima- und Umwelttestgeräte und andere
Temperatur-Konditionierungsgeräte
(IEC 61010-2-012:2019)

This European Standard was approved by CENELEC on 2019-05-17. CENELEC members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN-CENELEC Management Centre or to any CENELEC member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CENELEC member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CENELEC members are the national electrotechnical committees of Austria, Belgium, Bulgaria, Croatia, Cyprus, the Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, the Netherlands, Norway, Poland, Portugal, Republic of North Macedonia, Romania, Serbia, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.



European Committee for Electrotechnical Standardization
Comité Européen de Normalisation Electrotechnique
Europäisches Komitee für Elektrotechnische Normung

CEN-CENELEC Management Centre: Rue de la Science 23, B-1040 Brussels

EN IEC 61010-2-012:2022+A11:2022 (E)

European foreword

The text of document 66/687/FDIS, future edition 2 of IEC 61010-2-012, prepared by IEC/TC 66 "Safety of measuring, control and laboratory equipment" was submitted to the IEC-CENELEC parallel vote and approved by CENELEC as EN IEC 61010-2-012:2022.

The following dates are fixed:

- latest date by which the document has to be implemented at national level by publication of an identical national standard or by endorsement (dop) 2022-10-29
- latest date by which the national standards conflicting with the document have to be withdrawn (dow) 2025-04-29

This document supersedes EN 61010-2-012:2016 and all of its amendments and corrigenda (if any).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CENELEC shall not be held responsible for identifying any or all such patent rights.

This document has been prepared under a Standardization Request given to CENELEC by the European Commission and the European Free Trade Association.

Any feedback and questions on this document should be directed to the users' national committee. A complete listing of these bodies can be found on the CENELEC website.

Endorsement notice

The text of the International Standard IEC 61010-2-012:2019 was approved by CENELEC as a European Standard without any modification.

European foreword to amendment A11

This document (EN IEC 61010-2-012:2022/A11:2022) has been prepared by CLC/TC 66X "Safety of measuring, control, and laboratory equipment".

The following dates are fixed:

- latest date by which this document has to be implemented at national level by publication of an identical national standard or by endorsement (dop) 2023-03-28
- latest date by which the national standards conflicting with this document have to be withdrawn (dow) 2025-03-28

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CENELEC shall not be held responsible for identifying any or all such patent rights.

This document amends EN IEC 61010-2-012:2022.

This document has been prepared under a Standardization Request given to CENELEC by the European Commission and the European Free Trade Association, and supports essential requirements of EU Directive(s) / Regulation(s).

For relationship with EU Directive(s) / Regulation(s), see informative Annex ZZ, which is an integral part of this document.

Any feedback and questions on this document should be directed to the users' national committee. A complete listing of these bodies can be found on the CENELEC website.

Annex ZA (normative)

Normative references to international publications with their corresponding European publications

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

NOTE 1 When an International Publication has been modified by common modifications, indicated by (mod), the relevant EN/HD applies.

NOTE 2 Up-to-date information on the latest versions of the European Standards listed in this annex is available here: www.cenelec.eu.

Annex ZA of EN 61010-1:2010/A1:2019 is applicable with the following additions:

<u>Publication</u>	<u>Year</u>	<u>Title</u>	<u>EN/HD</u>	<u>Year</u>
IEC 60079-15	2010	<i>Explosive atmospheres – Part 15: Equipment protection by type of protection “n”</i>	EN 60079-15	2010
IEC 60079-20-1	-	<i>Explosive atmospheres – Part 20-1: Material characteristics for gas and vapour classification – Test methods and data</i>	EN 60079-20-1	2010
IEC 60335-2-34	2012	<i>Household and similar electrical appliances – Safety – Part 2–34: Particular requirements for motor-compressors</i>	EN 60335-2-34	2013
+ AMD1	2015		+ AMD1	2015
+ AMD2	2016		+ AMD2	2016
IEC 60950-1	2005	<i>Information technology equipment – Safety – Part 1: General requirements</i>	EN 60950-1	2006
ISO 7010		Graphical symbols - Safety colours and safety signs - Registered safety signs	EN ISO 7010	2020
		<i>Pumps and pump units for liquids - Common safety requirements</i>	EN 809 +A1	1998 2009
		<i>Pressure gauges - Part 1: Bourdon tube pressure gauges - Dimensions, metrology, requirements and testing</i>	EN 837-1	1996
		<i>Pressure gauges - Part 2: Selection and installation recommendations for pressure gauges</i>	EN 837-2	1997
		<i>Pressure gauges - Part 3: Diaphragm and capsule pressure gauges - Dimensions, metrology, requirements and testing</i>	EN 837-3	1996
		<i>Refrigerating systems and heat pumps - Flexible pipe elements, vibration isolators, expansion joints and non-metallic tubes - Requirements, design and installation</i>	EN 1736	2008
		<i>Non-destructive testing - Leak testing - Criteria for method and technique selection</i>	EN 1779 +A1	1999 2003 

EN IEC 61010-2-012:2022+A11:2022 (E)

 Publication	Year	Title	EN/HD	Year
		<i>Refrigerating systems and heat pumps - Liquid level indicating devices - Requirements, testing and marking</i>	EN 12178	2016
		<i>Refrigerating systems and heat pumps - Safety switching devices for limiting the pressure - Requirements and tests</i>	EN 12263	1998
		<i>Refrigerating systems and heat pumps - Valves - Requirements, testing and marking</i>	EN 12284	2003
		<i>Refrigerating systems and heat pumps - Safety and environmental requirements - Positive displacement refrigerant compressors</i>	EN 12693	2008
		<i>Refrigerating systems and heat pumps - Pressure relief devices and their associated piping - Methods for calculation</i>	EN 13136 +A1	2013 2018
		<i>Unfired pressure vessels - Part 1: General</i>	EN 13445-1 +A1 +A2	2014 2014 2018
		<i>Unfired pressure vessels - Part 2: Materials</i>	EN 13445-2 +A1 +A2 +A3	2014 2016 2018 2018
		<i>Unfired pressure vessels - Part 3: Design</i>	EN 13445-3 +A1 +A2 +A3 +A4 +A4 +A6 +A7 +A8	2014 2015 2016 2017 2018 2018 2019 2019 2019
		<i>Unfired pressure vessels - Part 4: Fabrication</i>	EN 13445-4 +A1	2014 2016
		<i>Unfired pressure vessels - Part 5: Inspection and testing</i>	EN 13445-5 +A1	2014 2018
		<i>Unfired pressure vessels - Part 6: Requirements for the design and fabrication of pressure vessels and pressure parts constructed from spheroidal graphite cast iron</i>	EN 13445-6 +A1 +A2	2014 2015 2018
		<i>Unfired pressure vessels - Part 8: Additional requirements for pressure vessels of aluminium and aluminium alloys</i>	EN 13445-8 +A1	2014 2014
		<i>Unfired pressure vessels - Part 10: Additional requirements for pressure vessels of nickel and nickel alloys</i>	EN 13445-10	2015
		<i>Metallic industrial piping - Part 1: General</i>	EN 13480-1 +A1	2017 2019



EN IEC 61010-2-012:2022/A11:2022 (E)

 Publication	Year	Title	EN/HD	Year
		<i>Metallic industrial piping - Part 2: Materials</i>	EN 13480-2	2017
			+A1	2018
			+A2	2018
			+A3	2018
			+A7	2018
		<i>Metallic industrial piping - Part 3: Design and calculation</i>	EN 13480-3	2017
			+A1	2021
			+A2	2020
			+A3	2020
		<i>Metallic industrial piping - Part 4: Fabrication and installation</i>	EN 13480-4	2017
		<i>Metallic industrial piping - Part 5: Inspection and testing</i>	EN 13480-5	2017
			+A1	2019
		<i>Metallic industrial piping - Part 6: Additional requirements for buried piping</i>	EN 13480-6	2017
			+A1	2018
		<i>Metallic industrial piping - Part 8: Additional requirements for aluminium and aluminium alloy piping</i>	EN 13480-8	2017
		<i>Pressure equipment for refrigerating systems and heat pumps - Part 1: Vessels - General requirements</i>	EN 14276-1	2006
			+A1	2013
		<i>Pressure equipment for refrigerating systems and heat pumps - Part 2: Piping - General requirements</i>	EN 14276-2	2007
			+A1	2013
		<i>Electric appliances connected to the water mains — Avoidance of back-siphonage and failure of hose-sets</i>	EN 61770	2009
			+A11	2018
IEC 60204-1		<i>Safety of machinery - Electrical equipment of machines - Part 1: General requirements</i>	EN 60204-1	2018
ISO 4126-1		<i>Safety devices for protection against excessive pressure - Part 1: Safety valves</i>	EN ISO 4126-1	2013
+A1			+A2	2019
ISO 4126-2		<i>Safety devices for protection against excessive pressure - Part 2: Bursting disc safety devices</i>	EN ISO 4126-2	2019



Annex ZZ
(informative)

Relationship between this European standard and the safety objectives of Directive 2014/35/EU [2014 OJ L96] aimed to be covered

This European Standard has been prepared under a Commission's standardization request relating to harmonized standards in the field of the Low Voltage Directive, M/511, to provide one voluntary means of conforming to safety objectives of Directive 2014/35/EU of the European Parliament and of the Council of 26 February 2014 on the harmonization of the laws of the Member States relating to the making available on the market of electrical equipment designed for use within certain voltage limits [2014 OJ L96].

Once this standard is cited in the Official Journal of the European Union under that Directive, compliance with the normative clauses of this standard given in Table ZZ.1 confers, within the limits of the scope of this standard, a presumption of conformity with the corresponding safety objectives of that Directive, and associated EFTA regulations.

Table ZZ.1 — Correspondence between this European standard and Annex I of Directive 2014/35/EU [2014 OJ L96]

Safety objectives of Directive 2014/35/EU (Annex I)	Clause(s) / subclause(s) of this EN	Remarks / Notes
1. General conditions		
1 (a) the essential characteristics, the recognition and observance of which will ensure that electrical equipment will be used safely and in applications for which it was made, shall be marked on the electrical equipment, or, if this is not possible, on an accompanying document	5.1 5.2 5.3 5.4	
1 (b) the electrical equipment, together with its component parts, shall be made in such a way as to ensure that it can be safely and properly assembled and connected	5.4 6.6 6.10 6.11, 11.101 Annex F	
1 (c) the electrical equipment shall be so designed and manufactured as to ensure that protection against the hazards set out in points 2 and 3 is ensured, providing that the equipment is used in applications for which it was made and is adequately maintained	5.4 Annex F 17 (for hazards not covered by Clauses 6 to 16) See also the details in points 2 and 3	

A11

A11

Safety objectives of Directive 2014/35/EU (Annex I)	Clause(s) / subclause(s) of this EN	Remarks / Notes
2. Protection against hazards arising from the electrical equipment Measures of a technical nature shall be laid down in accordance with point 1, in order to ensure that:		
2 (a) persons and domestic animals are adequately protected against the danger of physical injury or other harm which might be caused by direct or indirect contact	4, 6.1 – 6.11, 9.6, 11.6, 14.4 Annex D, Annex F, Annex K	
2 (b) temperatures, arcs or radiation which would cause a danger, are not produced	4, 4.4.4.2, 6.3.1.b) 2), 6.3.2 b) 2), 9.5, 9.6, 10.1 – 10.5, 10.101, 11.101, 12	
2 (c) persons, domestic animals and property are adequately protected against non-electrical dangers caused by the electrical equipment which are revealed by experience	4, 4.4, 7.2- 7.7, 9, 11 (with reference to Annex EE), 12.3, 12.5, 12.6, 13.1, 13.2, 16.2	
2 (d) the insulation is suitable for foreseeable conditions	4, 6.7, Annex K	
3. Protection against hazards which may be caused by external influences on the electrical equipment Technical measures shall be laid down in accordance with point 1, in order to ensure that the electrical equipment:		
3 (a) meets the expected mechanical requirements in such a way that persons, domestic animals and property are not endangered	4, 7, 8	
3 (b) is resistant to non-mechanical influences in expected environmental conditions, in such a way that persons, domestic animals and property are not endangered	1.4, 4, 6.7.2.2.1, 10.5, 10.102, 11.6, 14.3, 14.8, 14.101, 14.102, 15, Annex CC	
3 (c) does not endanger persons, domestic animals and property in foreseeable conditions of overload	4, 9, 14, 16.1, 16.101	

WARNING 1 — Presumption of conformity stays valid only as long as a reference to this European standard is maintained in the list published in the Official Journal of the European Union. Users of this standard should consult frequently the latest list published in the Official Journal of the European Union.

WARNING 2 — Other Union legislation may be applicable to the product(s) falling within the scope of this standard. A11

CONTENTS

FOREWORD	4
INTRODUCTION	7
1 Scope and object	10
2 Normative references	11
3 Terms and definitions	13
4 Tests	19
5 Marking and documentation	25
6 Protection against electric shock	34
7 Protection against mechanical HAZARDS	36
8 Resistance to mechanical stresses	38
9 Protection against the spread of fire	39
10 Equipment temperature limits and resistance to heat	40
11 Protection against HAZARDS from fluids and solid foreign objects	44
12 Protection against radiation, including laser sources, and against sonic and ultrasonic pressure	59
13 Protection against liberated gases and substances, explosion and implosion	60
14 Components and subassemblies	62
15 Protection by interlocks	64
16 HAZARDS resulting from application	66
17 RISK assessment	67
Annexes	68
Annex K (normative) Insulation requirements not covered by 6.7	69
Annex L (informative) Index of defined terms	70
Annex AA (informative) Useful symbols	72
Annex BB (informative) Protection of people who are inside WALK-IN EQUIPMENT	75
Annex CC (informative) Safety requirements for components and piping	77
Annex DD (informative) Equipment containing FLAMMABLE REFRIGERANTS – Information and marking requirements	82
Annex EE (normative) Non-sparking "n" electrical device	85
Bibliography	86
Figure 101 – Schema of a REFRIGERATING SYSTEM incorporating a CONDENSER	8
Figure 102 – Flow chart illustrating the selection process	9
Figure 103 – Details of scratching TOOL tip	54
Table 1 – Symbols	26
Table 101 – Time-temperature conditions	32
Table 102 – Maximum temperatures for MOTOR-COMPRESSORS	42
Table 103 – Minimum temperature for the determination of SATURATED-VAPOUR PRESSURE of the REFRIGERANT	49
Table 104 – REFRIGERANT flammability parameters	58
Table AA.1 – Useful symbols	

Table CC.1 – Parameters of pressure vessels according to EN 14276-1	77
Table CC.2 – Parameters of piping according to EN 14276-2.....	79
Table CC.3 – Components and piping requirements.....	80

INTERNATIONAL ELECTROTECHNICAL COMMISSION

**SAFETY REQUIREMENTS FOR ELECTRICAL EQUIPMENT
FOR MEASUREMENT, CONTROL, AND LABORATORY USE –****Part 2-012: Particular requirements for climatic and environmental
testing and other temperature conditioning equipment**

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

International Standard IEC 61010-2-012 has been prepared by IEC technical committee 66: Safety of measuring, control and laboratory equipment.

It has the status of a group safety publication in accordance with IEC Guide 104.

This second edition cancels and replaces the first edition published in 2016. This edition constitutes a technical revision.

This edition includes the following significant technical changes with respect to the previous edition:

- a) alignment with changes introduced by Amendment 1 of IEC 61010-1:2010;
- b) changes related to the use of small capitals for defined terms only;
- c) clarifications for cooling tests in 4.4.2.10;

- d) requirements for overtemperature protection in 10.101, including deletion of the second part of the sentence in item b), and the deletion of item c);
- e) changes pertaining to the accurate employment of terms "temperature", "operating temperature", "working temperature", "application temperature", "room temperature" and "ambient temperature" in 3.5.104, 3.5.105, 4.3.1, 4.3.2, 5.4.2, 8.2.1, 8.2.2, 11.7.2.101.2, 11.7.2.101.3, 13.2.102, 14.102, 15.101, 15.102, 15.103, Introduction and many other locations. For the purpose of clarification, the definition of 3.5.114, CONTROLLED TEMPERATURE, is added.

The text of this International Standard is based on the following documents:

FDIS	Report on voting
66/687/FDIS	66/688/RVD

Full information on the voting for the approval of this International Standard can be found in the report on voting indicated in the above table.

This document has been drafted in accordance with the ISO/IEC Directives, Part 2.

A list of all parts of the IEC 61010 series, published under the general title, *Safety requirements for electrical equipment for measurement, control, and laboratory use*, can be found on the IEC website.

IEC 61010-2-012 is to be used in conjunction with the latest edition of IEC 61010-1. It was established on the basis of the third edition (2010) and its Amendment 1 (2016), hereinafter referred to as Part 1.

This Part 2-012 supplements or modifies the corresponding clauses in IEC 61010-1 so as to convert that publication into the IEC standard: *Particular requirements for climatic and environmental testing and other temperature conditioning equipment*.

Where a particular subclause of Part 1 is not mentioned in this Part 2-012, that subclause applies as far as is reasonable. Where this Part 2-012 states "addition", "modification", "replacement", or "deletion", the relevant requirement, test specification, or note in Part 1 should be adapted accordingly.

In this standard:

- 1) the following print types are used:
 - requirements and definitions: in roman type;
 - NOTES: in smaller roman type;
 - *conformity and tests: in italic type*;
 - terms used throughout this standard which have been defined in Clause 3: SMALL ROMAN CAPITALS.
- 2) subclauses, figures, tables and notes which are additional to those in Part 1 are numbered starting from 101. Additional annexes are lettered starting from AA.

The committee has decided that the contents of this document will remain unchanged until the stability date indicated on the IEC website under "<http://webstore.iec.ch>" in the data related to the specific document. At this date, the document will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

IMPORTANT – The 'colour inside' logo on the cover page of this publication indicates that it contains colours which are considered to be useful for the correct understanding of its contents. Users should therefore print this standard using a colour printer.

INTRODUCTION

This Part 2-012, along with Part 2-010 and Part 2-011, taken together, address the specific HAZARDS associated with the heating and cooling of materials by equipment and are organized as follows:

IEC 61010-2-010	Specifically addresses the HAZARDS associated with equipment incorporating heating systems.
IEC 61010-2-011	Specifically addresses the HAZARDS associated with equipment incorporating REFRIGERATING SYSTEMS.
IEC 61010-2-012	Specifically addresses the HAZARDS associated with equipment incorporating both heating and REFRIGERATING SYSTEMS that interact with each other such that the combined heating and REFRIGERATING SYSTEM yield additional or more severe HAZARDS for the two systems than if treated separately. It also addresses the HAZARDS associated with the treatment of materials by other factors like irradiation, excessive humidity, CO ₂ and MECHANICAL MOVEMENT, etc.

Guidance for the application of the appropriate Part 2 standard(s)

When the equipment includes only a material heating system, and no REFRIGERATING SYSTEM or other environmental factors apply, then Part 2-010 applies without needing Part 2-011 or Part 2-012. Similarly, when the equipment includes only a REFRIGERATING SYSTEM, and no material heating system or other environmental factors apply, then Part 2-011 applies without needing Part 2-010 or Part 2-012. However, when the equipment incorporates both a material heating system, and a REFRIGERATING SYSTEM or the materials being treated in the intended application introduce significant heat into the REFRIGERATING SYSTEM, a determination should be made as to whether the interaction between the two systems will generate additional or more severe HAZARDS than if the systems were evaluated separately (CONTROLLED TEMPERATURE, see flow chart for selection process). If the interaction of the heating and cooling functions yields no additional or more severe HAZARDS, then both Part 2-010 and Part 2-011 apply for their respective functions. Conversely, if additional or more severe HAZARDS result from the combining of the heating and cooling functions, or if the equipment incorporates additional material treatment factors, then Part 2-012 applies, but not Part 2-010 or Part 2-011.

What HAZARDS are applicable for a REFRIGERATING SYSTEM?

The typical HAZARDS for a REFRIGERATING SYSTEM (see Figure 101) consisting of a MOTOR-COMPRESSOR, a CONDENSER, an expansion device and an EVAPORATOR include but are not limited to:

- The maximum temperature of LOW-PRESSURE SIDE (return temperature) to the MOTOR-COMPRESSOR. A MOTOR-COMPRESSOR incorporates a REFRIGERANT cooled motor and it should be established that the maximum temperatures of the LOW-PRESSURE SIDE under least favourable condition do not exceed the insulation RATINGS within the motor.
- The maximum pressure of LOW-PRESSURE SIDE at the inlet to the MOTOR-COMPRESSOR. The housing of the MOTOR-COMPRESSOR is exposed to this pressure and so the design RATING of the MOTOR-COMPRESSOR housing should accommodate the worst-case pressures whilst providing the correct safety margin for a pressure vessel.
- The maximum temperature of HIGH-PRESSURE SIDE to the CONDENSER. The temperatures of the HIGH-PRESSURE SIDE under most unfavourable conditions may present a temperature HAZARD if the OPERATOR is exposed to them or if the electrical insulation is degraded.
- The maximum pressure of HIGH-PRESSURE SIDE at the outlet to the MOTOR-COMPRESSOR. The REFRIGERANT components downstream of the MOTOR-COMPRESSOR up to the expansion device are exposed to this pressure and so the design RATING of these components should accommodate the worst-case pressures whilst providing the appropriate safety margin for a pressure vessel.

- The maximum CONTROLLED TEMPERATURES, namely, the SOAKED TEMPERATURE CONDITIONS, from which the heat is being extracted, may impact the maximum temperature of LOW-PRESSURE SIDE to the MOTOR-COMPRESSOR as well as present a temperature HAZARD if the OPERATOR is exposed to them or if the electrical insulation is degraded. Whether this CONTROLLED TEMPERATURE is derived from an integral heating function of the device or from the heat dissipated from the material being cooled, the impact under worst case conditions should be evaluated.
- The current draw of the equipment should be established when including the worst-case running conditions of the REFRIGERATING SYSTEM including any defrost cycles that may apply.

The worst-case conditions should be determined for the equipment and will include both the least favourable NORMAL USE conditions as well as the most unfavourable testing results under SINGLE FAULT CONDITIONS.


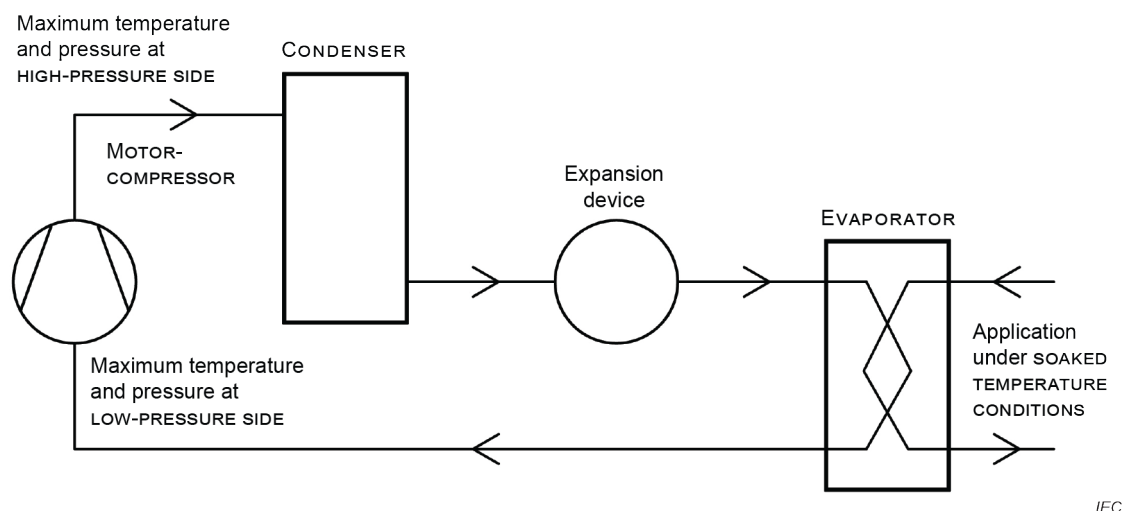


Figure 101 – Schema of a REFRIGERATING SYSTEM incorporating a CONDENSER

The selection process is illustrated in the following flow chart (see Figure 102).

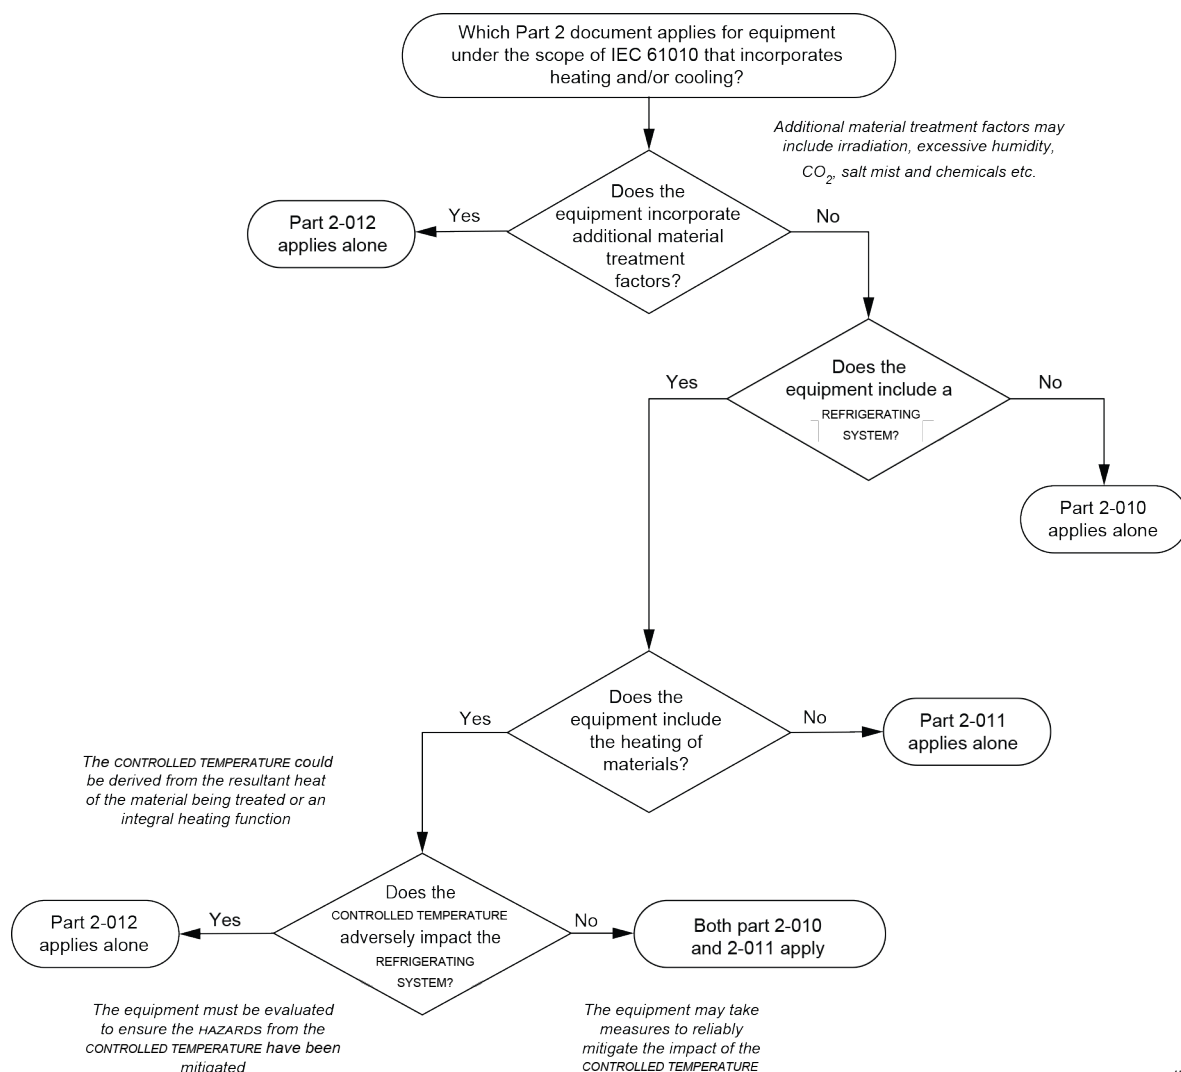

IEC

Figure 102 – Flow chart illustrating the selection process

SAFETY REQUIREMENTS FOR ELECTRICAL EQUIPMENT FOR MEASUREMENT, CONTROL AND LABORATORY USE –

Part 2-012: Particular requirements for climatic and environmental testing and other temperature conditioning equipment

1 Scope and object

This clause of Part 1 is applicable except as follows:

1.1.1 Equipment included in scope

Replacement:

Replace the second paragraph by the following:

This part of IEC 61010 specifies safety requirements for electrical equipment and its accessories within the categories a) through c), wherever it is intended to be used, whenever that equipment incorporates one or more of the following characteristics:

- A REFRIGERATING SYSTEM that is acted on or impacted by an integral heating function such that the combined heating and REFRIGERATING SYSTEM generates additional and/or more severe HAZARDS than those for the two systems if treated separately.
- The materials being treated in the intended application introduce significant heat into the REFRIGERATING SYSTEM, so that the REFRIGERATING SYSTEM in the application yields additional and/or more severe HAZARDS than those for the REFRIGERATING SYSTEM if operated at the maximum RATED ambient temperature alone.
- An irradiation function for the materials being treated presenting additional HAZARDS.
- A function to expose the materials being treated to excessive humidity, carbon dioxide, salt mist, or other substances which can result in additional HAZARDS.
- A function of MECHANICAL MOVEMENT presenting additional HAZARDS.
- Provision for an OPERATOR to walk in to the operating area to load or unload the materials being treated.

Addition:

Add the following text after the last paragraph:

NOTE 101 Examples of such equipment include environmental testing and plant growth TEST CHAMBERS, refrigerating CIRCULATORS which incorporate heating, and recirculating coolers for extracting heat.

It is possible that all or part of the equipment falls within the scope of one or more other Part 2 standards of IEC 61010 as well as within the scope of this standard. In that case, the requirements of those other Part 2 standards also apply. This document is intended for application when one or more of the additional HAZARDS described in the above dashed listed items are introduced. However, when the equipment incorporates only a REFRIGERATING SYSTEM or only a heating function or a combination of the two without introducing the additional HAZARDS described in the above list, then IEC 61010-2-011 or IEC 61010-2-010 or both, as appropriate, apply instead of this Part 2-012.

See further information in the flow chart (Figure 102) for selection process and guidance in the Introduction.

NOTE 102 Subclause 3.1.107 and Annex BB provide the definition and requirements for the protection of people who are inside WALK-IN EQUIPMENT.

1.1.2 Equipment excluded from scope

Addition:

Add the following items after item j):

- aa) equipment for the heating, cooling, and ventilation of laboratories;
- bb) sterilizing equipment.

1.2 Object

1.2.1 Aspects included in scope

Addition:

Add the following items after item g):

- aa) biohazards (see 13.101);
- bb) hazardous chemical substances (see 13.102).

2 Normative references

This clause of Part 1 is applicable, except as follows:

Addition:

IEC 60079-15:2010, *Explosive atmospheres – Part 15: Equipment protection by type of protection "n"*

IEC 60079-20-1, *Explosive atmospheres – Part 20-1: Material characteristics for gas and vapour classification – Test methods and data*

IEC 60335-2-34:2012, *Household and similar electrical appliances – Safety – Part 2-34: Particular requirements for motor-compressors*

IEC 60335-2-34:2012/AMD1:2015

IEC 60335-2-34:2012/AMD2:2016

IEC 60950-1:2005, *Information technology equipment – Safety – Part 1: General requirements*

ISO 7010, *Graphical symbols – Safety colours and safety signs – Registered safety signs* (available at <https://www.iso.org/obp>)

 EN 809, *Pumps and pump units for liquids - Common safety requirements*

EN 837-1, *Pressure gauges - Part 1: Bourdon tube pressure gauges - Dimensions, metrology, requirements and testing*

EN 837-2, *Pressure gauges - Part 2: Selection and installation recommendations for pressure gauges*

EN 837-3, *Pressure gauges - Part 3: Diaphragm and capsule pressure gauges - Dimensions, metrology, requirements and testing*

EN 1736, *Refrigerating systems and heat pumps - Flexible pipe elements, vibration isolators, expansion joints and non-metallic tubes - Requirements, design and installation*

EN 1779:1999, *Non-destructive testing - Leak testing - Criteria for method and technique selection*

EN 12178, *Refrigerating systems and heat pumps - Liquid level indicating devices - Requirements, testing and marking*

EN 12263, *Refrigerating systems and heat pumps - Safety switching devices for limiting the pressure - Requirements and tests*

EN 12284, *Refrigerating systems and heat pumps - Valves - Requirements, testing and marking*

EN 12693, *Refrigerating systems and heat pumps - Safety and environmental requirements - Positive displacement refrigerant compressors*

EN 13136, *Refrigerating systems and heat pumps - Pressure relief devices and their associated piping - Methods for calculation*

EN 13445-1, *Unfired pressure vessels - Part 1: General*

EN 13445-2, *Unfired pressure vessels - Part 2: Materials*

EN 13445-3, *Unfired pressure vessels - Part 3: Design*

EN 13445-4, *Unfired pressure vessels - Part 4: Fabrication*

EN 13445-5, *Unfired pressure vessels - Part 5: Inspection and testing*

EN 13445-6, *Unfired pressure vessels - Part 6: Requirements for the design and fabrication of pressure vessels and pressure parts constructed from spheroidal graphite cast iron*

EN 13445-8, *Unfired pressure vessels - Part 8: Additional requirements for pressure vessels of aluminium and aluminium alloys*

EN 13445-10, *Unfired pressure vessels - Part 10: Additional requirements for pressure vessels of nickel and nickel alloys*

EN 13480-1, *Metallic industrial piping - Part 1: General*

EN 13480-2, *Metallic industrial piping - Part 2: Materials*

EN 13480-3, *Metallic industrial piping - Part 3: Design and calculation* 

 EN 13480-4, *Metallic industrial piping - Part 4: Fabrication and installation*

EN 13480-5, *Metallic industrial piping - Part 5: Inspection and testing*

EN 13480-6, *Metallic industrial piping - Part 6: Additional requirements for buried piping*

EN 13480-8, *Metallic industrial piping - Part 8: Additional requirements for aluminium and aluminium alloy piping*

EN 14276-1, *Pressure equipment for refrigerating systems and heat pumps - Part 1: Vessels - General requirements*

EN 14276-2, *Pressure equipment for refrigerating systems and heat pumps - Part 2: Piping - General requirements*

EN 61770, *Electric appliances connected to the water mains - Avoidance of backsiphonage and failure of hose-sets*

IEC 60204-1, *Safety of machinery - Electrical equipment of machines - Part 1: General requirements*

ISO 4126-1, *Safety devices for protection against excessive pressure — Part 1: Safety valves*

ISO 4126-2, *Safety devices for protection against excessive pressure — Part 2: Bursting disc safety devices* 

3 Terms and definitions

This clause of Part 1 is applicable except as follows:

3.1 Equipment and states of equipment

Addition:

Add the following new terms and definitions:

3.1.101

BATH

complete device intended for application of CONTROLLED TEMPERATURES to SPECIMENS by immersion in a temperature-controlled liquid HEAT TRANSFER MEDIUM

3.1.102

CIRCULATOR

equipment intended for application of CONTROLLED TEMPERATURES to an APPLICATION SYSTEM by external circulating of a temperature-controlled liquid HEAT TRANSFER MEDIUM

3.1.103

TEST CHAMBER

ENCLOSURE or space in some part of which specified conditions can be achieved, in particular, temperature, humidity, irradiation, low air pressure, mould growth and salt spray

3.1.104

COMBINED TEST CHAMBER

special TEST CHAMBER combined with the function of MECHANICAL MOVEMENT, for example, for vibration, shock, impact, and similar dynamic tests

3.1.105

INCUBATOR

special TEST CHAMBER, primarily for incubation of microorganisms and tissue culture

3.1.106

SHAKER

equipment to disperse or dissolve one substance in another by MECHANICAL MOVEMENT without the use of blades or stirrers that might destroy the structure of the substance, in particular, shaking BATH and shaking INCUBATOR

3.1.107

WALK-IN EQUIPMENT

TEST CHAMBER or INCUBATOR, the door of which allows the OPERATOR to enter and remain inside the equipment even with the door closed

3.1.108

DRYING-OUT

period to wait or procedure to be carried out before operation to return the equipment to NORMAL CONDITION if it has been transported or stored in humid conditions, or moved from a cold environment to a much warmer one where condensation could occur, and could cause the equipment to then fail to meet all the safety requirements of this document

3.1.109

STANDSTILL

period to wait or procedure to be carried out before operation to return the equipment to NORMAL CONDITION if it has been transported, moved, shaken, tilted or inverted and which could cause the equipment to then fail to meet all the safety requirements of this document

3.2 Parts and accessories

Addition:

Add the following new terms and definitions:

3.2.101**RESISTANCE-HEATING DEVICE**

part of resistance-heating equipment, comprising one or more heating resistors, typically composed of metallic conductors or an electrically conductive compound suitably insulated and protected

[SOURCE: IEC 60050-426:2008, 426-08-08, modified – "resistance-heating unit" has been replaced with "resistance-heating equipment".]

3.2.102**REFRIGERATING SYSTEM**

combination of interconnected REFRIGERANT-containing parts constituting one closed REFRIGERANT circuit in which the REFRIGERANT is circulated for the purpose of extracting and rejecting heat

[SOURCE: ISO 5149-1:2014, 3.1.9, modified – the term "(heat pump)" has been deleted from the term and the words "(i.e. cooling and heating)" have been deleted from the definition and the note.]

3.2.103**CASCADE SYSTEM**

REFRIGERATING SYSTEM consisting of two or more independent refrigeration circuits where the CONDENSER of one system rejects heat directly to the EVAPORATOR of another

[SOURCE: EN 378-1:2008, 3.1.12, modified – "REFRIGERATING SYSTEM consisting of" has been included.]

3.2.104**MOTOR-COMPRESSOR**

refrigerating subassembly consisting of the mechanical mechanism of the compressor and the motor, both of which are enclosed in the same sealed housing, with no external shaft seals, and with the motor operating in a REFRIGERANT atmosphere with or without oil

Note 1 to entry: The housing may be permanently sealed, such as by welding or brazing (hermetic MOTOR-COMPRESSOR), or may be sealed by gasketed joints (semi-hermetic MOTOR-COMPRESSOR). A TERMINAL box, a TERMINAL boxcover, and other electrical components or an electronic control system may be included.

[SOURCE: IEC 60335-2-34:2012, 3.101, modified – "appliance" has been replaced by "refrigerating subassembly".]

3.2.105**CONDENSER**

heat exchanger in which vaporized REFRIGERANT is liquified by removal of heat

[SOURCE: ISO 5149-1:2014, 3.4.4, modified – "refrigerant vapour" has been replaced by "vaporized REFRIGERANT".]

3.2.106**CONDENSING UNIT**

specific refrigerating subassembly combination for a given REFRIGERANT, consisting of one or more MOTOR-COMPRESSORS, CONDENSERS, liquid receivers (when required) and the regularly furnished accessories

3.2.107**EVAPORATOR**

heat exchanger in which liquid REFRIGERANT is vaporized by absorption of heat

[SOURCE: IEC 60335-2-40:2018, 3.110, modified – "refrigerant liquid" has been replaced by "liquid refrigerant".]

3.2.108

HIGH-PRESSURE SIDE

part of a REFRIGERATING SYSTEM operating approximately at the CONDENSER pressure

[SOURCE: ISO 5149-1:2014, 3.1.7]

3.2.109

LOW-PRESSURE SIDE

part of a REFRIGERATING SYSTEM operating approximately at the EVAPORATOR pressure

[SOURCE: ISO 5149-1:2014, 3.1.8]

3.2.110

CIRCULATING PUMP

pressure and/or suction pump transporting the liquid HEAT TRANSFER MEDIUM in a BATH or CIRCULATOR

3.2.111

CIRCULATING FAN

propeller fan or centrifugal impeller designed to circulate the air in a TEST CHAMBER or an INCUBATOR with or without any air duct

3.2.112

HUMIDIFIER

electric device that generates a water mist or steam and releases it into a room, greenhouse or other ENCLOSURE

3.2.113

BATH TANK

open or enclosed vessel containing the HEAT TRANSFER MEDIUM, in a BATH or CIRCULATOR

3.2.114

LIQUID CONNECTION

pipe fitting through which liquid is expelled from or discharged into a vessel or a heat exchanger

3.2.115

VENTILATOR

device for replacing air inside a TEST CHAMBER or an INCUBATOR with outside air

3.2.116

TEMPERATURE-LIMITING DEVICE

temperature-actuated device that is designed to prevent unsafe temperatures

[SOURCE: EN 378-1:2008, 3.6.5]

3.2.117

LIQUID LEVEL CUT OUT

liquid level-actuated device designed to prevent unsafe liquid levels

[SOURCE: EN 378-1:2008, 3.6.12]

3.2.118

PRESSURE-LIMITING DEVICE

pressure-actuated device (for example, a high-pressure switch) which is designed to stop the operation of the pressure-imposing element and may also operate an alarm

3.2.119**PRESSURE-RELIEF DEVICE**

valve or disc designed to relieve excessive pressure automatically

[SOURCE: ISO 5149-1:2014, 3.6.7, modified – "pressure relief valve or bursting disc device" has been replaced with "valve or disc" in the definition.]

3.2.120**FLAMMABLE LIQUID**

liquid capable of producing a flammable gas or vapour which, when mixed with air in certain proportions, will form an EXPLOSIVE GAS ATMOSPHERE under any foreseeable operating conditions

3.2.121**HEAT TRANSFER MEDIUM**

medium used to transfer heat to the material being processed

3.2.122**REFRIGERANT**

fluid used for heat transfer in a REFRIGERATING SYSTEM, which absorbs heat at a low temperature and a low pressure of the fluid and rejects heat at a higher temperature and a higher pressure of the fluid, usually involving changes of state of the fluid

[SOURCE: ISO 817:2014, 3.1.35, modified – the term "phase" has been replaced with "state" in the definition.]

3.2.123**FLAMMABLE REFRIGERANT**

REFRIGERANT with a flammability classification of A2L, A2 or A3 in accordance with ISO 817

[SOURCE: IEC 60335-2-24:2010 and IEC 60335-2-24:2010/AMD2:2017, 3.109]

3.2.124**SPECIMEN**

any material, substance, or product designated to be processed, for example, in a BATH, TEST CHAMBER or an INCUBATOR

3.2.125**APPLICATION SYSTEM**

system or device intended to work with a CIRCULATOR to carry out a functional purpose

3.5 Safety terms

Addition:

Add the following new terms and definitions:

3.5.101**SATURATED-VAPOUR PRESSURE**

<of REFRIGERANT> vapour pressure at which the liquid and vapour can exist in equilibrium at a given temperature

3.5.102**MAXIMUM ALLOWABLE PRESSURE****PS**

maximum pressure for which the equipment is designed, as specified by the manufacturer

Note 1 to entry: This note applies to the French language only.

[SOURCE: EN 378-1:2008, 3.3.2]

3.5.103

RATED PRESSURE

MAXIMUM ALLOWABLE PRESSURE for pressure components of equipment with regard to their ability to withstand pressures as specified by the manufacturer

3.5.104

ACTIVE COOLING CONTROL RANGE

ACC RANGE

CONTROLLED TEMPERATURE range that is achieved by an active REFRIGERATING SYSTEM

Note 1 to entry: This note applies to the French language only.

3.5.105

FLASH POINT

lowest liquid temperature at which, under certain standardized conditions, a liquid gives off vapours in quantity such as to be capable of forming an ignitable vapour/air mixture

Note 1 to entry: At the FLASH POINT, the vapour may cease to burn when the ignition source is removed.

[SOURCE: IEC 60050-426:2008, 426-02-14]

3.5.106

FIRE POINT

lowest temperature at which a substance ignites and continues to burn for at least 5 s after a small flame has been applied to its surface under standardized conditions

3.5.107

AUTO IGNITION TEMPERATURE

lowest temperature at which a substance will spontaneously ignite in a normal atmosphere without an external ignition source, such as a flame or spark

Note 1 to entry: Once ignited, the substance will continue to burn until it is either completely consumed or the temperature of the remainder of the substance is reduced to or below its FIRE POINT.

3.5.108

LOWER EXPLOSIVE LIMIT

LEL

concentration of flammable gas or vapour in air, below which an EXPLOSIVE GAS ATMOSPHERE will not be formed

Note 1 to entry: This note applies to the French language only.

[SOURCE: IEC 60050-426:2008, 426-02-09]

3.5.109

EXPLOSIVE GAS ATMOSPHERE

mixture with air, under atmospheric conditions, of flammable substances in the form of gas or vapour which, after ignition, permits self sustaining flame propagation

[SOURCE: IEC 60050-426:2008, 426-01-07]

3.5.110

SOAKED TEMPERATURE CONDITION

temperature conditions when the ambient temperature of the equipment under test (EUT) equals to $\pm 2,0$ °C of maximum ambient of 1.4.1 for NORMAL USE, storage or transport, and the CONTROLLED TEMPERATURE of the EUT equals to $\pm 2,0$ °C of the maximum ACC RANGE with the MOTOR-COMPRESSOR running or, the maximum RATED CONTROLLED TEMPERATURE with the MOTOR-COMPRESSOR off

Note 1 to entry: This note applies to the French language only.

3.5.111

MECHANICAL MOVEMENT

motion of materials being processed, for example in a SHAKER or COMBINED TEST CHAMBER

3.5.112

MOVEMENT FREQUENCY

number of complete cycles of MECHANICAL MOVEMENT

3.5.113

MOVEMENT AMPLITUDE

maximum radius, distance, or angle of the MECHANICAL MOVEMENT

3.5.114

CONTROLLED TEMPERATURE

temperature where the EVAPORATOR is located and to which the LOW-PRESSURE SIDE of the equipment is exposed, as a result of heat transfer either by active heating or from the APPLICATION SYSTEM or SPECIMEN

Note 1 to entry: For a heat pump system, where a four-way valve is used to shift between heat and cool, the function of CONDENSER and EVAPORATOR is exchanged.

4 Tests

This clause of Part 1 is applicable except as follows:

4.3 Reference test conditions

4.3.1 Environmental conditions

Addition:

Add the following text after item d):

Since the temperatures, pressures and current draw for a REFRIGERATING SYSTEM are significantly impacted by ambient temperatures in a non-linear way, linear extrapolation of test data is not possible. Therefore, tests to establish the temperatures, pressures, and current draw for a REFRIGERATING SYSTEM shall be conducted under the following environmental conditions:

- 1) an ambient temperature of 40 °C, or the maximum RATED ambient temperature, if higher;
- 2) the temperature of water supply is the maximum as specified by the manufacturer (see 5.4.3);
- 3) a relative humidity not exceeding the limits of 1.4.1 d), or the maximum RATED relative humidity at the maximum RATED ambient temperature, if higher.

If, as permitted by Note 2 of 1.4.1, a REFRIGERATING SYSTEM has an ambient temperature RATING below 40 °C, the NORMAL CONDITION tests shall be performed in an environment that matches the maximum RATED ambient temperature, and then repeated at an ambient temperature of 40 °C. See 4.3.2.114.

4.3.2 State of equipment

4.3.2.1 General

Replacement:

Replace the first paragraph and note by the following:

Unless otherwise specified, each test shall be carried out on the equipment assembled for NORMAL USE, and under the least favourable combination of the conditions given in 4.3.2.2 to 4.3.2.13 and 4.3.2.101 to 4.3.2.114 if applicable.

When measuring temperatures, pressures, and current draws of equipment incorporating a REFRIGERATING SYSTEM, the tests shall be started from a SOAKED TEMPERATURE CONDITION when all pressures have fully equalized. Tests at the extremes of the input voltage ($\pm 10\%$) shall start under these voltage conditions and achieve a stable state but need not start from a SOAKED TEMPERATURE CONDITION.

In case of doubt, a test may have to be made with more than one combination of conditions, for example, when the equipment is operated at or cycled in between its maximum and minimum CONTROLLED TEMPERATURES or operated in combination with excessive humidity, low air pressure, radiation, or conditions of precipitation.

Addition:

Add the following new subclauses:

4.3.2.101 Heat load

Where the equipment or materials being processed require either the provision or extraction of heat, the equipment under test (EUT) shall be loaded with a heat source/sink within the manufacturer's specified conditions of use (including maximum RATED and none).

NOTE DIN 12876 (all parts) provides procedures for determining cooling capacity and efficient heating capacity of the equipment.

4.3.2.102 Humidity and steam

Where equipment generates humidity or is intended for connection to a steam supply, it shall be set to generate or be supplied with them within the manufacturer's specified conditions of use (including maximum RATED and none).

4.3.2.103 Lamp and lamp systems

Illumination that provides part of the primary function (whether it be integral or an accessory), shall be installed and operated within the manufacturer's specified conditions of use (including maximum, off and cycled).

NOTE An example is a Xenon arc lamp used in a weather durability TEST CHAMBER.

4.3.2.104 MECHANICAL MOVEMENT

Equipment with a function of MECHANICAL MOVEMENT (for materials or HEAT TRANSFER MEDIUM) shall be set to expose the equipment and any materials being processed to the worst conditions (including maximum, off and cycled).

4.3.2.105 Spray generating systems

Spray generating systems of equipment shall be operated within the manufacturer's specified conditions of use (including maximum, off and cycled).

4.3.2.106 VENTILATORS

VENTILATORS shall be operated within the manufacturer's specified conditions of use (including maximum, off and cycled).

4.3.2.107 Pressures other than those of REFRIGERANT

Where equipment generates or uses pressures other than local atmospheric it shall be set to generate, or be supplied with pressure(s) within the manufacturer's specified conditions of use (including maximum RATED and none).

4.3.2.108 REFRIGERANT pressure

Where a heating system (or HEAT TRANSFER MEDIUM) can apply a CONTROLLED TEMPERATURE to the REFRIGERATING SYSTEM which is outside its ACC RANGE, the equipment shall be set to apply the maximum CONTROLLED TEMPERATURE allowed by the controls or interlocks with the MOTOR-COMPRESSOR off or maximum ACC RANGE with the MOTOR-COMPRESSOR on, whichever is least favourable.

Where a heating system (or HEAT TRANSFER MEDIUM) can apply a CONTROLLED TEMPERATURE to the REFRIGERATING SYSTEM which could affect the pressure in the system, the most unfavourable condition for pressure shall be established including:

- MOTOR-COMPRESSOR running throughout;
- MOTOR-COMPRESSOR started during test;
- outside its ACC RANGE with the MOTOR-COMPRESSOR off and the equipment set to apply the maximum CONTROLLED TEMPERATURE allowed by the controls or interlocks.

4.3.2.109 Exhaust and condensate

The least favourable conditions which result in production of exhaust, vapours and/or condensates shall be created (including maximum and cycled).

NOTE The TERMINALS of a RESISTANT-HEATING DEVICE exposed to ambient condition are easily condensed after the HEAT TRANSFER MEDIUM has been cooled to below ambient temperature for some time.

4.3.2.110 Filling and draining systems

Filling and draining systems shall be operated within the manufacturer's specified conditions of use (including maximum, minimum and intermediate).

4.3.2.111 Circulating system

CIRCULATING PUMP(s), agitator(s) or CIRCULATING FAN(s) shall be operated within the manufacturer's specified conditions of use (including maximum and off).

4.3.2.112 Gas HEAT TRANSFER MEDIUM

The equipment shall be operated with the gas HEAT TRANSFER MEDIUM, whether it is air or other designated gases, at the percentage of content and pressure within the manufacturer's specified conditions of use (including maximum, minimum and none).

4.3.2.113 Properties of liquid HEAT TRANSFER MEDIUM

For equipment with a wide CONTROLLED TEMPERATURE range, the effect of contraction, expansion, evaporating, condensing, oxidizing, boiling and freezing of the liquid and its allowable CONTROLLED TEMPERATURE range should be considered. HEAT TRANSFER MEDIA which change states during NORMAL USE shall be simulated to generate state change both from solid to liquid and vice versa.

4.3.2.114 Abnormal test to simulate the failure of the controlled environment

For REFRIGERATING SYSTEMS intended to operate in an ambient environment that is more restricted than that specified in 1.4.1, this additional abnormal test shall be applied to simulate the failure of the controlled environment in which the equipment is located