

Health informatics — Point-of-care medical device communication —

**Part 30200: Transport profile — Cable
connected**

ICS 35.240.80

National foreword

This British Standard is the UK implementation of EN ISO 11073-30200:2005+A1:2015. It supersedes BS EN ISO 11073-30200:2005, which is withdrawn. It is identical to ISO/IEEE 11073-30200:2004, incorporating amendment 1:2015.

The start and finish of text introduced or altered by amendment is indicated in the text by tags. Tags indicating changes to ISO text carry the number of the ISO amendment. For example, text altered by ISO amendment 1 is indicated by A1 A1.

The UK participation in its preparation was entrusted to Technical Committee IST/35, Health informatics.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 28 April 2006

© The British Standards Institution 2015.
Published by BSI Standards Limited 2015

ISBN 978 0 580 86143 7

Amendments/corrigenda issued since publication

Date	Comments
31 December 2015	Implementation of ISO/IEEE amendment 1:2015

English Version

Health informatics - Point-of-care medical device communication
- Part 30200: Transport profile - Cable connected (ISO/IEEE
11073-30200:2004)

Informatique de santé - Communication entre dispositifs
médicaux sur le site des soins - Partie 30200: Profil de
transport - Connexion par câble (ISO/IEEE 11073-
30200:2004)

Medizinische Informatik - Kommunikation patientennaher
medizinischer Geräte - Teil 30200: Transportprofil -
drahtgebundene Übertragung

This European Standard was approved by CEN on 16 August 2005.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: rue de Stassart, 36 B-1050 Brussels

BS EN ISO 11073-30200:2005+A1:2015

EN ISO 11073-30200:2005+A1:2015

Foreword

The text of ISO/IEEE 11073-30200:2004 has been prepared by Technical Committee ISO/TC 215 "Health informatics" of the International Organization for Standardization (ISO) and has been taken over as EN ISO 11073-30200:2005 by Technical Committee CEN/TC 251 "Health informatics", the secretariat of which is held by NEN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by February 2006, and conflicting national standards shall be withdrawn at the latest by February 2006.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.

Endorsement notice

The text of ISO/IEEE 11073-30200:2004 has been approved by CEN as EN ISO 11073-30200:2005 without any modifications.

Foreword to amendment 1

The text of ISO 11073-30200:2004/Amd1:2015 has been prepared by Technical Committee ISO/TC 215 "Health informatics" of the International Organization for Standardization (ISO) and has been taken over as EN ISO 11073-30200:2005/A1:2015 by Technical Committee CEN/TC 251 "Health informatics" the secretariat of which is held by NEN.

This Amendment to the European Standard EN ISO 11073-30200:2005 shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by March 2016, and conflicting national standards shall be withdrawn at the latest by March 2016.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

According to the CEN-CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.

Endorsement notice

The text of ISO 11073-30200:2004/Amd 1:2015 has been approved by CEN as EN ISO 11073-30200:2005/A1:2015 without any modification.

BS EN ISO 11073-30200:2005+A1:2015
ISO 11073-30200:2005+A1:2015

IEEE Standards documents are developed within the IEEE Societies and the Standards Coordinating Committees of the IEEE Standards Association (IEEE-SA) Standards Board. The IEEE develops its standards through a consensus development process, approved by the American National Standards Institute, which brings together volunteers representing varied viewpoints and interests to achieve the final product. Volunteers are not necessarily members of the Institute and serve without compensation. While the IEEE administers the process and establishes rules to promote fairness in the consensus development process, the IEEE does not independently evaluate, test, or verify the accuracy of any of the information contained in its standards.

Use of an IEEE Standard is wholly voluntary. The IEEE disclaims liability for any personal injury, property or other damage, of any nature whatsoever, whether special, indirect, consequential, or compensatory, directly or indirectly resulting from the publication, use of, or reliance upon this, or any other IEEE Standard document.

The IEEE does not warrant or represent the accuracy or content of the material contained herein, and expressly disclaims any express or implied warranty, including any implied warranty of merchantability or fitness for a specific purpose, or that the use of the material contained herein is free from patent infringement. IEEE Standards documents are supplied “**AS IS**.”

The existence of an IEEE Standard does not imply that there are no other ways to produce, test, measure, purchase, market, or provide other goods and services related to the scope of the IEEE Standard. Furthermore, the viewpoint expressed at the time a standard is approved and issued is subject to change brought about through developments in the state of the art and comments received from users of the standard. Every IEEE Standard is subjected to review at least every five years for revision or reaffirmation. When a document is more than five years old and has not been reaffirmed, it is reasonable to conclude that its contents, although still of some value, do not wholly reflect the present state of the art. Users are cautioned to check to determine that they have the latest edition of any IEEE Standard.

In publishing and making this document available, the IEEE is not suggesting or rendering professional or other services for, or on behalf of, any person or entity. Nor is the IEEE undertaking to perform any duty owed by any other person or entity to another. Any person utilizing this, and any other IEEE Standards document, should rely upon the advice of a competent professional in determining the exercise of reasonable care in any given circumstances.

Interpretations: Occasionally questions may arise regarding the meaning of portions of standards as they relate to specific applications. When the need for interpretations is brought to the attention of IEEE, the Institute will initiate action to prepare appropriate responses. Since IEEE Standards represent a consensus of concerned interests, it is important to ensure that any interpretation has also received the concurrence of a balance of interests. For this reason, IEEE and the members of its societies and Standards Coordinating Committees are not able to provide an instant response to interpretation requests except in those cases where the matter has previously received formal consideration. At lectures, symposia, seminars, or educational courses, an individual presenting information on IEEE standards shall make it clear that his or her views should be considered the personal views of that individual rather than the formal position, explanation, or interpretation of the IEEE.

Comments for revision of IEEE Standards are welcome from any interested party, regardless of membership affiliation with IEEE. Suggestions for changes in documents should be in the form of a proposed change of text, together with appropriate supporting comments. Comments on standards and requests for interpretations should be addressed to:

Secretary, IEEE-SA Standards Board
445 Hoes Lane
P.O. Box 1331
Piscataway, NJ 08855-1331 USA

NOTE — Attention is called to the possibility that implementation of this standard may require use of subject matter covered by patent rights. By publication of this standard, no position is taken with respect to the existence or validity of any patent rights in connection therewith. The IEEE shall not be responsible for identifying patents for which a license may be required by an IEEE standard or for conducting inquiries into the legal validity or scope of those patents that are brought to its attention.

Authorization to photocopy portions of any individual standard for internal or personal use is granted by the Institute of Electrical and Electronics Engineers, Inc., provided that the appropriate fee is paid to Copyright Clearance Center. To arrange for payment of licensing fee, please contact Copyright Clearance Center, Customer Service, 222 Rosewood Drive, Danvers, MA 01923 USA; +1 978 750 8400. Permission to photocopy portions of any individual standard for educational classroom use can also be obtained through the Copyright Clearance Center.

ISO Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75% of the member bodies casting a vote.

A pilot project between ISO and the IEEE has been formed to develop and maintain a group of ISO/IEEE standards in the field of medical devices as approved by Council resolution 43/2000. Under this pilot project, IEEE is responsible for the development and maintenance of these standards with participation and input from ISO member bodies.

Attention is drawn to the possibility that some of the elements of this International Standard may be the subject of patent rights. Neither ISO nor the IEEE shall be held responsible for identifying any or all such patent rights.

ISO/IEEE 11073-30200:2004(E) was prepared by IEEE 1073 Committee of the IEEE Engineering in Medicine and Biology Society.

IEEE Introduction

This introduction is not part of ISO/IEEE 11073-30200:2004(E), Health informatics — Point-of-care medical device communication — Part 30200: Transport profile — Cable connected.

ISO/IEEE 11073 standards enable communication between medical devices and external computer systems. They provide automatic and detailed electronic data capture of patient vital signs information and device operational data. The primary goals are to:

- Provide real-time plug-and-play interoperability for patient-connected medical devices
- Facilitate the efficient exchange of vital signs and medical device data, acquired at the point-of-care, in all health care environments

“Real-time” means that data from multiple devices can be retrieved, time correlated, and displayed or processed in fractions of a second. “Plug-and-play” means that all the clinician has to do is make the connection — the systems automatically detect, configure, and communicate without any other human interaction.

“Efficient exchange of medical device data” means that information that is captured at the point-of-care (e.g., patient vital signs data) can be archived, retrieved, and processed by many different types of applications without extensive software and equipment support, and without needless loss of information. The standards are especially targeted at acute and continuing care devices, such as patient monitors, ventilators, infusion pumps, ECG devices, etc. They comprise a family of standards that can be layered together to provide connectivity optimized for the specific devices being interfaced.

ISO/IEEE 11073-30200:2004(E) defines a communications transport profile. This profile is for a cable-connected local area network (LAN) for the interconnection of computers and medical devices. This standard is suitable for new device designs, but is particularly targeted to modifications of legacy devices.

The term “legacy devices” refers to equipment that is

- Already in use in clinical facilities
- In active production at the facilities of medical device manufacturers, or
- Beyond the initial stages of engineering development

Specifically, this standard describes connection-oriented communications services and protocols consistent with standards of the Infrared Data Association (IrDA), adapted as appropriate for ISO/IEEE 11073 applications and optimized for use in patient-connected bedside medical devices.

ISO/IEEE 11073-30200:2004(E) is one part of the family of ISO/IEEE 11073 standards. It is compatible with the upper layer ISO/IEEE 11073 standards.

The primary users of this standard are technical personnel who are creating or interfacing with a medical device communications system. Familiarity with the ISO/IEEE 11073 family of standards is recommended. Familiarity with communications and networking technologies is also recommended.

This standard is intended to satisfy the following objectives:

- a) Allow compatibility with existing medical device communications designs to minimize design risk, contain product costs, and simplify field upgrades
- b) Specify hardware and software elements that are available from multiple vendors
- c) Make use of other computer industry communication technology to allow for continuous cost decreases
- d) Meet the requirements of IEEE Std 1073™-1996
- e) Be compatible with the current published and draft ISO/IEEE standard upper layers

Notice to users

Patents

Attention is called to the possibility that implementation of this standard may require use of subject matter covered by patent rights. By publication of this standard, no position is taken with respect to the existence or validity of any patent rights in connection therewith. The IEEE shall not be responsible for identifying patents or patent applications for which a license may be required by to implement an IEEE standard or for conducting inquiries into the legal validity or scope of those patents that are brought to its attention.

Errata

Errata, if any, for this and all other standards can be accessed at the following URL: <http://standards.ieee.org/reading/ieee/updates/errata/index.html>. Users are encouraged to check this URL for errata periodically.

Interpretations

Current interpretations can be accessed at the following URL: <http://standards.ieee.org/reading/ieee/interp/index.html>.

Participants

At the time this guide was completed, the Legacy Device Working Group of the IEEE 1073 Committee had the following membership:

Allen Farquhar, *Chair*

Todd Cooper
Kenneth J. Fuchs
Harald Greiner

Kenneth Hall
Dick Myrick
Daniel Nowicki
Paul Schluter

Ward Silver
Lars Steubesand
Jan Wittenber

Other individuals who have contributed to this document include

Frank Enslin
George Kriegl

Tom Luteran

Bob Meijer
Carol Pellegrini

The following members of the balloting committee voted on this standard:

Teresa J. Cendrowska
Allen Farquhar
Ricardo Ruiz Fernandez
Kenneth J. Fuchs

Harald Greiner
Bill Hawley
Debra Herrmann
Robert J. Kennelly
William McMullen

Daniel Nowicki
Melvin Reynolds
M. Michael Shabot
Lars Steubesand

BS EN ISO 11073-30200:2005+A1:2015
ISO 11073-30200:2005+A1:2015

When the IEEE-SA Standards Board approved this standard on 30 January 2000, it had the following membership:

Richard J. Holleman, *Chair*
Donald N. Heirman, *Vice Chair*
Judith Gorman, *Secretary*

Satish K. Aggarwal
Dennis Bodson
Mark D. Bowman
James T. Carlo
Gary R. Engmann
Harold E. Epstein
Jay Forster*
Ruben D. Garzon

James H. Gurney
Lowell G. Johnson
Robert J. Kennelly
E. G. “Al” Kiener
Joseph L. Koepfinger*
L. Bruce McClung
Daleep C. Mohla
Robert F. Munzner

Louis-François Pau
Ronald C. Petersen
Gerald H. Peterson
John B. Posey
Gary S. Robinson
Akio Tojo
Hans E. Weinrich
Donald W. Zipse

*Member Emeritus

Also included is the following nonvoting IEEE-SA Standards Board liaison:

Robert E. Hebner

Yvette Ho Sang
Don Messina
IEEE Standards Project Editors

CONTENTS

1.	Overview.....	1
1.1	Scope.....	2
1.2	Purpose.....	2
1.3	Standards compatibility	2
1.4	Audience	2
2.	References.....	2
3.	Definitions, acronyms, and abbreviations.....	4
3.1	Definitions	4
3.2	Acronyms and abbreviations	6
4.	Goals for this standard	7
A1	4.1 Compliance with other standards A1	7
5.	Architecture	8
5.1	Topology.....	8
5.2	Layering.....	9
6.	Physical layer.....	10
7.	Data link layer.....	10
7.1	IrLAP frame.....	11
7.2	Procedure model	12
7.3	Minimum data link layer requirements.....	13
8.	Network layer	16
8.1	Discovery information	16
8.2	Information access requirements	18
8.3	Minimum IrLMP multiplexer requirements	20
9.	Transport layer.....	21
9.1	Maximum transfer unit	21
9.2	Transport service requirements.....	22
9.3	MDDL service	23
10.	Time synchronization	23
11.	Labeling and conformance requirements.....	24
11.1	Labeling requirements	24
11.2	Conformance requirements.....	24
	Annex A (normative) Physical layer.....	25
	Annex B (informative) Maximum cable length	36
	Annex C (informative) Modular connectors	38

BS EN ISO 11073-30200:2005+A1:2015
ISO 11073-30200:2005+A1:2015

Annex D (informative) RJ-45 to DB-9 modular adapters	40
Annex E (informative) Detailed rationale for pin assignments	41
Annex F (informative)  10BASE-T/100BASE-TX of IEEE Std 802.3-2008 	42
Annex G (informative) Power delivery considerations	43
Annex H (informative) Nonisolated BCC and DCC design examples	44
Annex I (informative) Isolated BCC design example	46
Annex J (informative) Optical isolator design example	48
Annex K (informative) Marking guidelines	50
Annex L (informative) IrDA message examples	53
Annex M (normative) IrDA profile	59
Annex N (informative) Time synchronization using SNTP	62
 Annex O (informative) Analysis of compatibility between ISO/IEEE Std 11073-30200:2004 and 10BASE-T/100BASE-TX of IEEE Std 802.3-2008 	70
Bibliography	96

Health informatics — Point-of-care medical device communication — Part 30200: Transport profile — Cable connected

1. Overview

 This standard is divided into 11 clauses, as follows:

- Clause 1 provides an overview of this standard.
- Clause 2 lists references to other standards that are useful in applying this standard.
- Clause 3 provides definitions and abbreviations.
- Clause 4 provides goals for this standard.
- Clause 5 provides an overview of network topology and layering.
- Clause 6 provides a profile of the physical layer.
- Clause 7 provides a profile of the data link layer.
- Clause 8 provides a profile of the network layer.
- Clause 9 provides a profile of the transport layer.
- Clause 10 describes the optional time synchronization service.
- Clause 11 provides labeling and conformance requirements.

This standard also contains 16 annexes, as follows:

- Annex A describes the physical layer.
- Annex B provides information on the maximum cable length.
- Annex C provides examples of physical link media.
- Annex D provides example schematics for modular adapters.
- Annex E provides a detailed rationale for pin assignments.
- Annex F describes the use of IEEE 802.3 10BASE-T/100BASE-TX with this standard.
- Annex G provides a discussion of power delivery considerations.
- Annex H provides examples of simple bedside communications controller (BCC) and device communications controller (DCC) designs.
- Annex I provides an example of an isolated BCC design.
- Annex J provides an optical isolator design example.
- Annex K provides marking guidelines.
- Annex L provides protocol examples, particularly of connection establishment.
- Annex M defines the Infrared Data Association (IrDA) profile specifications adapted from the IrDA implementation guidelines. 

BS EN ISO 11073-30200:2005+A1:2015

ISO 11073-30200:2005+A1:2015

- A1)** — Annex N provides guidelines for using the SNTP time synchronization protocol.
- Annex O provides an analysis of compatibility between ISO/IEEE Std 11073-30200:2004 and 10BASE-T/100BASE-TX of IEEE Std 802.3-2008 [B10].
- Annex P provides bibliographical references. **A1)**

1.1 Scope

The scope of this standard is an IrDA-based, cable-connected local area network (LAN) for the interconnection of computers and medical devices. This standard is suitable for new device designs, but is particularly targeted to modifications of legacy devices.

The term “legacy devices” refers to equipment that is

- Already in use in clinical facilities
- In active production at the facilities of medical device manufacturers, or
- Beyond the initial stages of engineering development

In each of these cases, the degree of effort to add a standardized communications capability might normally be prohibitive, unless special care is taken in developing a suitable standard.

1.2 Purpose

The purpose of this standard is to provide connection-oriented communications services and protocols consistent with IrDA specifications and adapted as appropriate for ISO/IEEE 11073 applications.

1.3 Standards compatibility

This standard is one part of the family of ISO/IEEE 11073 standards. It is compatible with the ISO/IEEE upper layer standards.

1.4 Audience

The primary users of this standard are technical personnel who are creating or interfacing with a medical device communications system. Familiarity with the ISO/IEEE 11073 family of standards is recommended. Familiarity with communications and networking technologies is also recommended.

2. References

This standard shall be used in conjunction with the following publications. When the following standards are superseded by an approved revision, the revision shall apply.

ANSI/TIA/EIA-232-F-1997, Interface Between Terminal Equipment and Data Circuit-Terminating Equipment Employing Serial Binary Data Interchange.¹

ANSI/TIA/EIA-561-1990, Simple 8 Position Non-Synchronous Interface Between Data Terminal Equipment and Data Circuit-Terminating Equipment Employing Serial Binary Data Interchange.

¹ANSI publications are available from the Sales Department, American National Standards Institute, 25 West 43rd Street, 4th Floor, New York, NY 10036, USA (<http://www.ansi.org/>).

ANSI/TIA/EIA-562-1989, Electrical Characteristics for an Unbalanced Digital Interface.

ANSI/TIA/EIA-568-A-1995, Commercial Building Telecommunications Cabling Standard.

IEC 60603-7: 1996, Connectors for Frequencies Below 3 MHz for Use with Printed Circuit Boards—Part 7: Detailed specification for connectors, 8-way, including fixed and free connectors with common mating features, with assessed quality.²

IEC 60417-1:1998, Graphical Symbols for Use on Equipment—Part 1: Overview and Application.

IEEE Std 802.3TM, IEEE Standard for Local Area Networks—Carrier Sense Multiple Access with Collision Detection (CSMA/CD) Access Method and Physical Layer Specifications.^{3, 4}

IEEE Std 1073TM-1996, IEEE Standard for Medical Device Communications—Transport Profiles—Overview and Framework.

IEEE Std 1073.3.1TM-1994, IEEE Standard for Medical Device Communications—Transport Profile—Connection Mode.⁵

IEEE Std 1073.4.1TM-1994, IEEE Standard for Medical Device Communications—Physical Layer Interface—Cable Connected.⁶

IrDA, Link Management Protocol, Version 1.1, Jan. 23, 1996.⁷

IrDA, Serial Infrared Link Access Protocol (IrLAP), Version 1.1, June 16, 1996.

IrDA, Tiny TP: A Flow-Control Mechanism for use with IrLMP, Version 1.1, Oct. 20, 1996.

ISO/IEC 8877:1992(E), Information technology—Telecommunications and information exchange between systems—Interface connector and contact assignments for ISDN Basic Access Interface located at reference points S and T.

RFC-1305, Internet Engineering Task Force, Network Working Group Report, Mar. 1992, “Network Time Protocol Specification, Implementation and Analysis,” Mills, D., University of Delaware.^{8, 9}

RFC-2030, Internet Engineering Task Force, Network Working Group Report, Oct. 1996, “Simple Network Time Protocol (SNTP) Version 4 for IPv4, IPv6 and OSI,” Mills, D., University of Delaware.

²IEC publications are available from the Sales Department of the International Electrotechnical Commission, Case Postale 131, 3, rue de Varembe, CH-1211, Genève 20, Switzerland/Suisse (<http://www.iec.ch/>). IEC publications are also available in the United States from the Sales Department, American National Standards Institute, 11 West 42nd Street, 13th Floor, New York, NY 10036, USA.

³IEEE publications are available from the Institute of Electrical and Electronics Engineers, 445 Hoes Lane, P.O. Box 1331, Piscataway, NJ 08855-1331, USA (<http://www.standards.ieee.org/>).

⁴The IEEE standards or products referred to in this clause are trademarks of the Institute of Electrical and Electronics Engineers, Inc.

⁵IEEE Std 1073.3.1-1994 has been withdrawn; however, copies can be obtained from Global Engineering, 15 Inverness Way East, Englewood, CO 80112-5704, USA, tel. (303) 792-2181 (<http://global.ihs.com/>).

⁶IEEE Std 1073.4.1-1994 has been withdrawn; however, copies can be obtained from Global Engineering, 15 Inverness Way East, Englewood, CO 80112-5704, USA, tel. (303) 792-2181 (<http://global.ihs.com/>).

⁷IrDA publications are available at <http://www.irda.org>.

⁸Internet Engineering Task Force publications are available at <http://www.ietf.org/>.

⁹Information on the Network Time Protocol is available at <http://www.eecis.udel.edu/~ntp/>.

3. Definitions, acronyms, and abbreviations

3.1 Definitions

^{A1} For the purposes of this document, the following terms and definitions apply. *The IEEE Standards Dictionary: Glossary of Terms & Definitions* should be consulted for terms not defined in this clause.²

Note that numerous definitions and abbreviations from IEEE Std 802.3–2008 [B10] are used in this document. Those definitions and abbreviations will not be repeated here. For specific information, please refer to Section One, subclause 1.4 and subclause 1.5, of IEEE Std 802.3-2008.

10BASE-T: IEEE Std 802.3-2008, physical layer specification for Ethernet over two pairs of unshielded twisted-pair (UTP) media at 10 Mb/s.

100BASE-TX: IEEE Std 802.3-2008 specifies operation over two copper media: two pairs of shielded twisted-pair cable (STP) and two pairs of unshielded twisted-pair cable (Category 5 UTP). For the purposes of this standard, only UTP is permitted. ^{A1}

baud: A unit of signaling speed, expressed as the number of times per second the signal can change the electrical state of the transmission line or other medium.

NOTE—Depending on the encoding strategies, a signal event may represent a single bit, more, or less, than one bit.

bedside communications controller (BCC): A communications controller, typically located at a patient bedside, that serves to interface between one or more medical devices. The BCC may be embedded into local display, monitoring, or control equipment. Alternatively, it may be part of a communications router to a remote hospital host computer system.

beginning of frame (BOF): An octet specified by infrared link access protocol (IrLAP).

category 5 (CAT-5) balanced cable: The designation applied to 100 Ω unshielded twisted-pair (UTP) cables and associated connecting hardware whose transmission characteristics are specified up to 100 MHz. (ANSI/TIA/EIA-568-A-1995)

cyclic redundancy check (CRC): The result of a calculation carried out on the octets within an IrLAP frame; also called a frame check sequence. The CRC is appended to the transmitted frame. At the receiver, the calculation creating the CRC may be repeated, and the result compared to that encoded in the signal. *Syn:* **frame check sequence**.

device communications controller (DCC): A communications interface associated with a medical device. A DCC may support one or more physically distinct devices acting as a single network communications unit. Its purpose is to provide a point-to-point serial communication link to a BCC.

electromagnetic compatibility (EMC): The ability of a device, equipment, or system to function satisfactorily in its electromagnetic environment without introducing intolerable electromagnetic disturbances to anything in that environment.

electromagnetic interference (EMI): Signals emanating from external sources (e.g., power supplies, transmitters) or internal sources (e.g., adjacent electronic components, energy sources) that disrupt or prevent operation of electronic systems.

^{A1} ² The IEEE Standards Dictionary: Glossary of Terms & Definitions is available at <http://standards.ieee.org>. ^{A1}

electrostatic discharge (ESD): The sudden transfer of charge between bodies of differing electrostatic potentials that may produce voltages or currents that could destroy or damage electrical components.

frame check sequence: *See:* cyclic redundancy check.

high-level data link control (HDLC): A standard protocol defined by ISO for bit-oriented, frame-delimited data communications.

information access service (IAS): A component of infrared link management protocol (IrLMP).

local area network (LAN): A communication network to interconnect a variety of intelligent devices (e.g., personal computers, workstations, printers, file storage devices) that can transmit data over a limited area, typically within a facility.

medical information bus (MIB): The informal name for the ISO/IEEE 11073 family of standards.

octet: A group of eight adjacent bits.

primary station: As defined by the infrared link access protocol (IrLAP), the station on the data link that assumes responsibility for the organization of data flow and for unrecoverable data link error conditions. It issues commands to the secondary stations and gives them permission to transmit.

protocol data unit (PDU): Information delivered as a unit between peer entities that contains control information and, optionally, data.

quality of service (QoS): The four negotiated parameters for a link: signaling speed, maximum turn-around time, data size, and disconnect threshold.

radio frequency (RF): (A) (Loosely) The frequency in the portion of the electromagnetic spectrum that is between the audio-frequency portion and the infrared portion. **(B)** A frequency useful for radio transmission.

NOTE—The present practicable limits of radio frequency are roughly 10 kHz to 100 000 MHz. Within this frequency range, electromagnetic radiation may be detected and amplified as an electric current at the wave frequency.¹⁰

radio frequency interference (RFI): *See:* radio interference.

radio interference: Degradation of the reception of a wanted signal caused by radio frequency (RF) disturbance.

NOTES

1—RF disturbance is an electromagnetic disturbance having components in the RF range.

2—The words “interference” and “disturbance” are often used indiscriminately. The expression “radio frequency interference” is also commonly applied to an RF disturbance or an unwanted signal.

RJ-45: (A) AT&T Registered Jack designation for the eight-pin modular connectors that meet the requirements of IEC 60603-7:1996 and ISO/IEC 8877:1992. **(B)** An eight-pin modular telephone plug.

NOTES

1—Also called a programmable connection, an RJ-45 plug is generally used on four-wire circuits, but can be used on eight-wire circuits.

2—Definition (B) reflects colloquial usage. Standards referencing this term should point to the precise standardized connector specification.

¹⁰ Notes in text, tables, and figures are given for information only and do not contain requirements needed to implement the standard.

BS EN ISO 11073-30200:2005+A1:2015

ISO 11073-30200:2005+A1:2015

RS-232: The serial interface defined in ANSI/TIA/EIA-232-F-1997.

secondary station: As defined by the infrared link access protocol (IrLAP), any station on the data link that does not assume the role of the primary station. It will initiate transmission only as a result of receiving explicit permission to do so from the primary station.

service access point (SAP): An address that identifies a user of the services of a protocol entity.

service data unit (SDU): Information that is delivered as a unit between peer service access points (SAPs). See: service access point.

set normal response mode (SNRM): A high-level data link control (HDLC) message sent by a bedside communications controller (BCC) to a device communications controller (DCC) when a successful connection to the network has occurred.

3.2 Acronyms and abbreviations

API	application program interface
AWG	American Wire Gage
BCC	bedside communications controller
BOF	beginning of frame
BPWR	bedside communications controller power
CAT-5	category 5
CRC	cyclic redundancy check
CS	connection sense
DCC	device communications controller
DPWR	device communications controller power
DTE	data terminal equipment
DTR	data terminal ready
EMC	electromagnetic compatibility
EMI	electromagnetic interference
EOF	end of frame
ESD	electrostatic discharge
EUI	extended unique identifier
GND	ground
HDLC	high-level data link control
IAS	information access service
IrDA	Infrared Data Association; the set of infrared data communications standards
IrLAP	IrDA link access protocol
IrLMP	IrDA link management protocol
IV	intravenous
LAN	local area network
LED	light-emitting diode
LI	leap indicator
LSAP	link service access point
LSB	least significant bit
MDDL	medical device data language
MIB	medical information bus
MSB	most significant bit
MTU	maximum transfer unit
NIBP	non-invasive blood pressure
NTP	network time protocol
 PoC	point of care 
PLL	phase-locked loop

PDU	protocol data unit
QoS	quality of service
RAC	IEEE Registration Authority Committee
RD	receive data
RF	radio frequency
RFI	radio frequency interference
RJ	registered jack
RR	receive ready
RTS	request to send
RxD	receive data
SAP	service access point
SAR	segmentation and reassembly
SDLC	synchronous data link control
SDU	service data unit
SNRM	set normal response mode
SNTP	simple network time protocol
TD	transmit data
TinyTP	tiny transport protocol
TTPSAP	TinyTP service access point
TxD	transmit data
UTC	coordinated universal time
UTP	unshielded twisted pair
XID	exchange station identification
XMIT	transmitting
VN	version number

4. Goals for this standard

The following are the main goals for this standard:

- The standard shall allow the use of existing RS-232 port designs to minimize design risk, contain product costs, and simplify field upgrades.
- The standard shall specify hardware and software elements that are available from multiple vendors.
- The standard should make use of other computer industry communication technology to allow for continuous cost decreases.
- The standard should meet the requirements of IEEE Std 1073-1996.
- The standard should be compatible with the current published and draft IEEE/ANSI standard upper layers.

4.1 Compliance with other standards

Devices that comply with this standard may also be required to comply with other domain- and device specific standards that supersede the requirements of this standard and IEEE Std 802.3-2008 [B10] to which this standard refers with respect to issues including safety, reliability, and risk management. A user of this standard is expected to be familiar with all other such standards that apply and to comply with any higher specifications thus imposed. Typically, medical devices will comply with the IEC 60601-1:2005 [B6] base standards and its parts, such as IEC 60601-1-1:2000 [B7], with respect to electrical and mechanical safety and any device specific standard as might be defined in IEC 60601-1-2:2007 [B8]. Software aspects may apply through standards such as EN 62304:2005 [B5]. 

BS EN ISO 11073-30200:2005+A1:2015

ISO 11073-30200:2005+A1:2015

A1 Devices that comply with this standard shall implement higher layers of network software as appropriate to the application. The requirements on performance of such applications and conformance are defined elsewhere and are outside the scope of this standard. Additionally, the network environment within which devices operate should be specified. Use of any medical equipment within a network environment shall be subject to risk assessment and risk management appropriate to the application and use and should adhere to standards such as ISO 14971:2007 [B11] and IEC 80001-1:2010 [B9]. The requirements of such risk assessment and risk management and conformance are outside the scope of this standard. **A1**

5. Architecture

This clause is intended to define ISO/IEEE 11073-30200 network topology and protocol layering.

5.1 Topology

The ISO/IEEE 11073-30200 network defines a star topology, requiring each device to have its own connection directly into the network. On the communications network, two types of communications nodes are allowed:

- The BCC is the primary node and functions as the network controller and the hub of the star.
- DCCs are secondary nodes and limited in number to the loading capacity of the BCC and/or number of physical port sockets.

The devices connect to the network through the DCC. The BCC can interface directly to a local host computer, as in Figure 1, or to a remote host computer over a network, as in Figure 2. The portion of the BCC performing ISO/IEEE 11073-30200 operations would be the same in both configurations. However, the BCC would also include internet-working functions in the latter case.

Unless otherwise noted, all references to a BCC in this standard refer only to the components performing ISO/IEEE 11073-30200 functions, as indicated in Figure 1 and Figure 2.

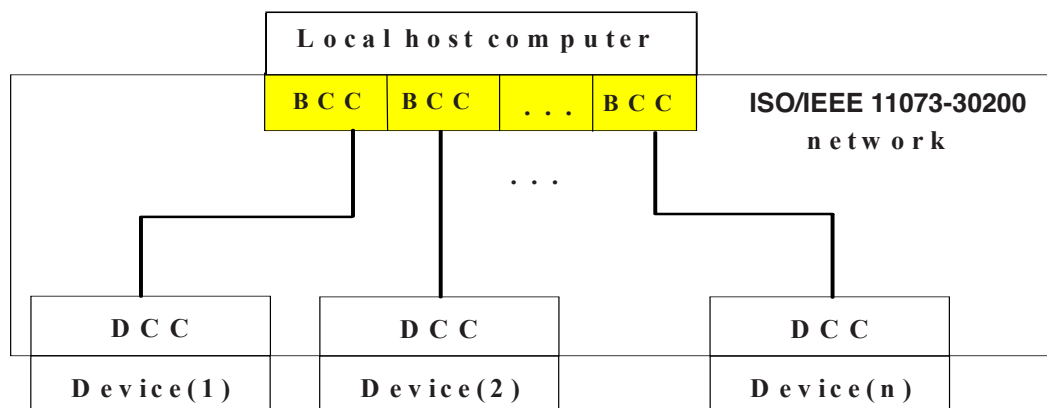


Figure 1 — Connection topology with a local host

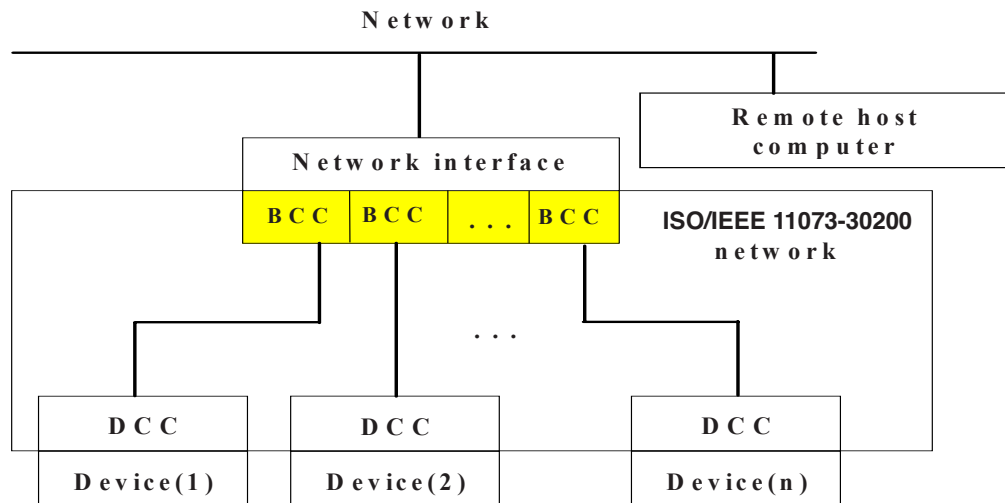


Figure 2—Connection topology with a remote host

The cable-connected network described by this standard consists of individual point-to-point connections between the BCC and each DCC: it is not a multidrop network. Only a single DCC is supported on each physical port connection.

5.2 Layering

Layering is consistent with the IrDA standards, as shown in Figure 3.

Briefly, the components of the stack are as follows.

- Physical layer, defining a standard connector and electrical characteristics (see Clause 6)
- Infrared link access protocol (IrLAP), providing a device-to-host connection for the reliable, ordered transfer of data, including device discovery procedures (see Clause 7)
- Infrared link management protocol (IrLMP), providing multiplexing of the IrLAP layer (see Clause 8)
- Tiny transport protocol (TinyTP), providing flow control on IrLMP connections (see Clause 9)
- Simple network time protocol (SNTTP) service access point (SAP), a SAP for an optional time synchronization service (see Clause 10)
- Medical device data languages (MDDL) SAP, as described in other ISO/IEEE 11073 standards

Related ISO OSI layer	ISO/IEEE 11073-30200 layer	
	SNTP SAP	MDDL SAP
Transport	Tiny transport protocol – TinyTP	
Network	Link management protocol - IrLMP	
Data link	Link access protocol – IrLAP	
Physical link	Physical layer	

Figure 3—ISO/IEEE 11073-30200 layering

Service primitives are specified for some of the layers. This definition of service does not imply any specific interface implementation. These primitives do not constitute an application program interface (API). Conformance to this standard is judged by performance at the communications port only.

6. Physical layer

The physical layer provides point-to-point connection sensing, data transmission and power delivery between the BCC and DCC using an eight-pin RJ-45 modular connector. The physical layer requirements are defined in Annex A.

Refer to the following additional informative annexes for more information about the physical layer:

- Annex B provides information on the maximum cable length.
- Annex C provides examples of physical link media.
- Annex D provides example schematics for modular adapters.
- Annex E provides a detailed rationale for pin assignments.
- [A1]** — Annex F describes the use of 10BASE-T/100BASE-TX with this standard. **[A1]**
- Annex G provides a discussion of power delivery considerations.
- Annex H provides examples of simple BCC and DCC designs.
- Annex I provides an example of an isolated BCC design.
- Annex J provides an optical isolator design example.
- Annex K provides marking guidelines.

7. Data link layer

The data link layer is adopted from the IrLAP, which implements ISO/OSI layer 2, the data link layer. It is based on standard asynchronous high-level data link control (HDLC) and synchronous data link control (SDLC) half-duplex protocols.

IrLAP provides the following features:

- a) Dynamic address and address conflict resolution
- b) Error recovery mechanism

- c) Station discovery and identification procedure
- d) Connectionless and connection-oriented services
- e) Negotiation of connection characteristics

This standard follows some of the recommendations of IrDA Lite [B4] for IrLAP. IrLAP capabilities not specified here are out of scope for an ISO/IEEE 11073-30200 interface. Examples of these capabilities are sniffing, connectionless data transfer, test frames, role exchange, and 2400 Bd operation.

IrLAP communication partners act in one of two roles: one primary station and one or more secondary stations. The primary station discovers all available secondary stations and establishes a connection to specific stations. The primary station is always the initiator of data transfer; the secondary station reacts to commands from the primary.

As shown in Figure 4, a BCC performs the functions of a primary station, and a DCC performs the functions of a secondary station. Although IrLAP supports multidrop communications in the infrared medium, this standard defines a single DCC at each cable-connected port on the BCC. Each port on a BCC represents a separate instance of the transport profile stack.

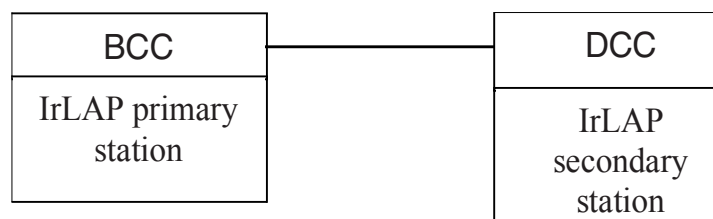


Figure 4—Logical network model

7.1 IrLAP frame

IrLAP defines a physical layer frame wrapper and a data link frame. The physical layer uses the ASYNC frame wrapper. The ASYNC frame wrapper has beginning frame (BOF), ending frame (EOF), and field check sequence fields. This frame encloses the data link frame, shown in Figure 5. IrLAP defines a transparency algorithm that allows the use of the framing characters (BOF and EOF) inside the data frame.



Figure 5—IrLAP frame

7.2 Procedure model

The simplified procedure model in Figure 6 illustrates the different procedures within an IrDA communication.

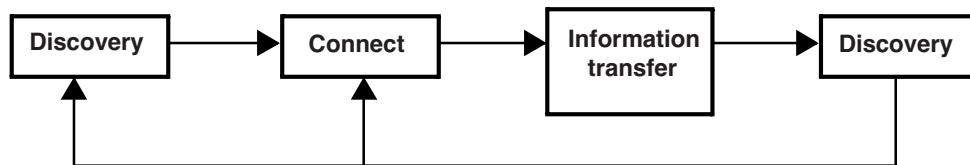


Figure 6— IrDA communication procedure model

7.2.1 Discovery

A primary station (the initiator) performs a discovery procedure to detect all available secondary devices. The secondary device (the responder) responds with address information and minimal device information (service hints and a device nickname). The discovery phase is done with a fixed set of communication parameters (e.g., 9600 Bd).

Discovery begins when the initiator broadcasts a discovery command frame. This command frame specifies the number of time slots for the discovery process—more time slots means more devices can be discovered and reduces the likelihood of collisions between responders during discovery.

Because this standard specifies a cable-connected topology, there is a maximum of one responder at each BCC port. In order to minimize the time spent during discovery, the BCC should provide only a single time slot for this procedure.

7.2.2 Negotiation and connection

The primary station establishes a connection by negotiating the maximum communication capabilities (e.g., signaling speed, data size, window size) supported by both devices. In the case of the BCC, this quality of service (QoS) may be constrained by available system bandwidth and the bandwidth requirements at other ports on the BCC.

After acknowledgement from the secondary station, both stations switch to the new communication parameters.

7.2.3 Information transfer

The primary station periodically polls the secondary station for data or status information. The stations communicate using a reliable data transport service. Stations may also use an unreliable expedited data transport service for time synchronization.

7.2.4 Disconnect

Both stations, primary or secondary, can normally disconnect the connection. In addition, timeout mechanisms on both sides detect a broken or aborted connection. All communication parameters are reset to negotiation values upon disconnect.

7.3 Minimum data link layer requirements

The minimum data link layer services support the capabilities of device discovery, connection, data transfer, and disconnection.

7.3.1 Minimum data link layer services

The status of the data link layer service primitives provided by a BCC or DCC is specified in Table 1 as follows:

M: Mandatory
C: Conditional

Table 1 — Data link layer service requirements

Service primitives	Status	
	BCC	DCC
Device discovery		
IrLAP_Discovery.request(gen addr bit)	M	N/A
IrLAP_Discovery.confirm(list of discovery logs)	M	N/A
IrLAP_Discovery.indication(discovery log)	N/A	M
Connection		
IrLAP_Connect.request(target device address, requested QoS, sniff ^a)	M	C ^b
IrLAP_Connect.confirm(connection handle, returned QoS)	M	C ^b
IrLAP_Connect.indication(source device addr, connection handle, returned QoS)	C ^b	M
IrLAP_Connect.response(source device addr, connection handle, requested QoS)	C ^b	M
Data transfer		
IrLAP_Data.request(connection handle, user data, expedited unreliable flag = false)	M	M
IrLAP_Data.indication(connection handle, user data, expedited unreliable flag = false)	M	M
IrLAP_Data.request(connection handle, user data, expedited unreliable flag = true)	C ^c	C ^c
IrLAP_Data.indication(connection handle, user data, expedited unreliable flag = true)	C ^c	C ^c
Disconnection		
IrLAP_Disconnect.request(connection handle)	M	M
IrLAP_Disconnect.indication(connection handle, unacked data)	M	M

^aUse of the sniffing feature is out of the scope of this standard.

^bIndicated connect services are required in a BCC or DCC that supports SNTP.

^cThe expedited unreliable IrLAP_Data services are required for the LM_UData/TTP_UData service in a BCC or DCC that supports SNTP.

7.3.2 Wrapping layer

Asynchronous framing and transparency shall be used, as defined by IrLAP.

7.3.3 Negotiation

At a minimum, the IrLAP negotiation parameters in Table 2 shall be supported.

Table 2—IrLAP minimum negotiation parameters

Signaling speed	9600 Bd
Maximum turnaround time	500 ms
Data size ^a	64 octets
Window size	1 frame window
Additional BOFs	0 BOFs
Link disconnect time	3 s
Link threshold time	0 s

^aThe data size parameter is the maximum number of data octets allowed in any received frame. A data size parameter of 64 octets is required for negotiation. A larger data size may also be required to support the range of transfer protocol data unit (PDU) sizes provided by this profile.

7.3.4 Link disconnect time

IrLAP supports the negotiation of the link disconnect time, i.e., the time a station will wait without receiving valid frames before it disconnects the link. IrLAP stations may support a variety of link disconnect times, ranging from 3 s to 40 s. An ISO/IEEE 11073-30200 station should exclusively support the minimum value for the link disconnect time of 3 s. A longer disconnect timeout might be useful for devices using an infrared medium, but is not necessary for a cable-connected device. The minimum disconnect time is preferred, in order to permit rapid identification of the disconnected state.

7.3.5 Contention state

In the contention state, 11 BOFs shall be used on every frame. The first 10 BOFs shall be FFh. The eleventh BOF shall be C0h.

7.3.6 Signaling speed

A station shall operate at 9600 Bd. A station may operate at other signaling speeds supported by IrLAP that use asynchronous framing: 19 200 Bd, 38 400 Bd, 57 600 Bd, or 115 200 Bd.

7.3.7 Data size

The maximum size of a PDU is negotiated at the time of the connection. The IrLAP “data size” parameter is negotiated independently for each direction of the link; therefore, the primary and secondary stations may support different maximum PDU sizes.

The negotiated signaling speed and turnaround time may constrain the actual data size by limiting the amount of time available to transfer the frame. If the requested data size cannot be supported, the link shall be renegotiated.

7.3.8 Poll interval

When a BCC transmits an information frame, IrLAP permits the turnaround time to be as short as the negotiated minimum turnaround time.

When a BCC has no information frame to transmit, it shall wait for some interval before issuing a “receive ready” poll frame. The polling interval is not specified in IrLAP, but shall be bounded by the negotiated minimum and maximum turnaround times. Maximum turnaround time shall be negotiated as shown in Table 3. IrLAP does not provide a mechanism for negotiating the polling interval, represented by the P-Timer-Expired event in the XMIT state of the primary role state machine.

Many applications of medical information bus (MIB) may expect the DCC to consume the bulk of the available bandwidth at low signaling speeds. If the BCC were to frequently wait for 500 ms to issue a poll frame, a substantial proportion of the potential bandwidth would go unused. If the BCC were to simply issue a poll frame after the minimum turnaround time, it could drive the device to spend an inordinate amount of time servicing an inactive communications link. Therefore, it is reasonable to allow the negotiation of an intermediate polling interval that optimizes bandwidth usage without interfering with device performance.

A DCC may advertise the preference to be polled at a shorter interval than 500 ms. The available selections are shown in Table 4. The preferred polling interval is advertised through the information access service (IAS) (see Clause 8).

BCCs shall poll at the maximum turnaround time unless a shorter polling interval is advertised by the DCC. A BCC shall not poll faster than the advertised polling interval. A BCC shall not poll faster than the minimum turnaround time. A polling interval of 0 ms means that the DCC will accept polling as fast as the minimum turnaround time.

NOTE—Selecting a shorter poll interval should not interfere with the maximum turnaround time that determines the time allotted to the DCC to transmit.

Table 3—Maximum turnaround time

Signaling speed (Bd)	Timing
9600	Stations are restricted to a fixed maximum turnaround time of 500 ms.
19 200	
38 400	
57 600	
115 200	Stations select a maximum turnaround time during negotiation.

Table 4—Polling interval selections

0 ms
50 ms
100 ms
250 ms

8. Network layer

The network link layer is adopted from the IrLMP, which implements ISO/OSI layer 3.

IrLMP consists of the following components:

- a) IAS maintains an information base with information about offered services and device information.
- b) Link management multiplexer provides multiple connections over IrLAP.

This standard follows some of the recommendations of IrDA Lite [B4] for IrLMP. IrLMP capabilities not specified here are out of scope for an ISO/IEEE 11073-30200 interface. Examples of these capabilities are sniffing, connectionless data transfer, and exclusive mode.

8.1 Discovery information

IrLMP as service user for the IrLAP services provides the discovery information shown in Figure 7. This information is a maximum of 23 octets long.




Figure 7—Discovery information field

Service hints are mandatory and contain at least 1 octet. They provide information about the general device class (e.g., computer, printer, modem). More hint octets can be appended to the first one. An ISO/IEEE 11073-30200 BCC or DCC shall assert the reserved service hint bit 12 and the extension bit 7, as shown in Table 5.

Table 5—Service hint bit assignment

Octet 1		Octet 2	
Bit	Function	Bit	Function
0		8	
1		9	
2		10	
3		11	
4		12	ISO/IEEE 11073 = 1
5		13	
6		14	
7	Extension = 1	15	

Not all IrDA devices that assert hint bit 12 are assured of supporting this standard. To be certain, the primary station should query the IAS of the secondary station for the IEEE:1073:3:2 object class (described in 8.2.6).

A BCC or DCC shall report a device nickname with the discovery information. The device nickname should be a short, recognizable name for the device. That name shall begin with the acronym “MIB” followed by a space. The format of the device nickname encoding is shown in Figure 8. This encoding shall include a character set code, as described in IrLMP. Examples of device nicknames are shown in Table 6.

Character set code (1 octet)	Name
---------------------------------	------

Figure 8—Device nickname format

Table 6—Sample device nicknames

Name	Encoding	Octets	Length
“MIB IV Pump”	ASCII	00 4D 49 42 20 49 56 20 50 75 6D 70	12 octets
“MIB Ventilator”	ASCII	00 4D 49 42 20 56 65 6E 74 69 6C 61 74 6F 72	15 octets
“MIB NIBP”	ASCII	00 4D 49 42 20 4E 49 42 50	9 octets
NOTE—IrLAP restricts the length of the discovery information (device nickname plus service hints) to 23 octets.			

8.2 Information access requirements

The information access requirements support the capabilities of a global identifier number, node type identification, and dynamic access point identification.

8.2.1 IAS

The IAS shall provide the service primitives described in Table 7. The status of an IAS primitives is specified as follows:

M: Service is mandatory
R: Service is recommended

Table 7—IAS requirements

IAS primitives	Status
LM_GetValueByClass.request(address, class name, attribute name)	M
LM_GetValueByClass.confirm(list of (object id, attribute value))	M
LM_GetValue.request(address, id, attribute name1, [attribute name2, ...])	R
LM_GetValue.confirm(list of attribute values)	R

8.2.2 Global identifier number

A BCC or DCC should report a global identifier number in the IAS object database, as shown in Table 8. The global identifier number is the 64 b global identifier [64 b extended unique identifier (EUI-64)] parameter for that BCC or DCC. This parameter consists of a 3-octet (24 b) company identifier (company_id) number followed by a 5-octet (40 b) extension identifier. The format, shown in Figure 9, follows the IrLMP conventions for an octet sequence.

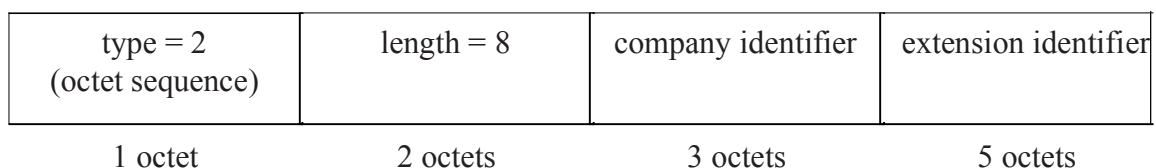


Figure 9—Global identifier format in IAS

The individual company_id number is assigned by the IEEE Registration Authority Committee (RAC) and represents a unique code for a particular manufacturing company or other organization.

The 40 b extension identifier number is assigned by the particular manufacturer or other organization. It is the responsibility of the individual manufacturer to assign a unique (nonduplicate) extension identifier number to each BCC or DCC.

No more than one 64 b global identifier value shall be contained within each component that is manufactured. For legacy devices that use a communications protocol adapter, the global identifier can reside in the adapter.

The use of the EUI-64 global identification number enables unique global identification of ISO/IEEE 11073 communication controllers. This identification allows for distinguishing between multiple devices of the same type that are connected to the same patient and facilitates device tracking and maintenance within an institution.

8.2.3 Interface type

A BCC or DCC shall report the type of interface supported (BCC or DCC) using the NodeType attribute as shown in Table 8 and Table 9.

8.2.4 Port identifier number

A BCC or DCC shall report a unique port number value for each port on the device, as described in Table 8 and Table 9.

8.2.5 Service access points

A BCC should specify a service connection endpoint for the SNTP upper layers to an IrDA TinyTP service, as shown in Table 8.

A DCC shall specify a service connection endpoint for the MDDL upper layers to an IrDA TinyTP service, as shown in Table 9.

8.2.6 Supported objects and attributes

The IAS in a BCC or DCC shall support the objects and attributes listed in Table 8 and Table 9, respectively. The status of an object-attribute pair is specified as follows:

- M: IAS entry is mandatory
- R: IAS entry is recommended
- O: IAS entry is optional

Table 8—Objects and attributes in a BCC

Object class	Attribute name	Value type	Description	Status
Device	DeviceName	user string	This attribute is described in IrLMP.	M
	IrLMPSupport	octet sequence	This attribute is described in IrLMP.	M
IEEE :1073:3:2	GlobalID	octet sequence	Specifies the global identifier number for the BCC.	R ^a
	NodeType	integer	0 (= BCC)	M
	PortNumber	integer	Ascribes a specific number to each port on the BCC.	M
IEEE :1073:3:2 :SNTP	IrDA:TinyTP :LsapSel	integer	Specifies the service connection endpoint for the SNTP upper layers to an IrDA TinyTP service.	R ^a

^aIf the capability is not supported, the attribute shall be omitted from the IAS.

Table 9—Objects and attributes in a DCC

Object class	Attribute name	Value type	Description	Status
Device	DeviceName	user string	This attribute is described in IrLMP.	M
	IrLMPSupport	octet sequence	This attribute is described in IrLMP.	M
IEEE :1073:3:2	GlobalID	octet sequence	Specifies the global identifier number for the DCC.	R ^a
	NodeType	integer	1 (= DCC)	M
	PortNumber	integer	Ascribes a specific number to each MIB DCC port on the medical device.	M
	PollInterval	integer	Specifies the preferred polling interval, in milliseconds. May be 0, 50, 100, or 250.	O ^a
IEEE :1073:3:2 :MDDL	IrDA:TinyTP :LsapSel	integer	Specifies the service connection end-point for the ISO/IEEE 11073 MDDL upper layers to an IrDA TinyTP service.	M

^aIf the capability is not supported, the attribute shall be omitted from the IAS.

8.2.7 Extending the list of objects and attributes

The objects and attributes supported by the IAS may be extended by other ISO/IEEE 11073 family standards. A standard that provides IAS extensions shall specify the object class, the attribute name, and the value type. The object class name should incorporate the name of the standard, as in “IEEE:1073:3:2”.

Reasons for extending the IAS include the possibility of providing a link service access point (LSAP) that uses a protocol other than MDDL or SNTP. The use of other LSAPs to establish connections to other services is out of the scope of this standard.

NOTE—If sessions are established on other LSAPs concurrent with MDDL, it is important to understand the impact of this connection on the throughput and latency performance of the MDDL connection. It may be necessary to service the MDDL connection at a higher priority in order to guarantee the desired level of throughput and/or latency. If SNTP is implemented, that link should be serviced as high-priority, low-latency. The impact of SNTP on throughput is negligible.

8.3 Minimum IrLMP multiplexer requirements

The minimum multiplexer requirements provide support for device discovery, connection, status, data transfer, and disconnection.

The network layer shall provide the service primitives described in Table 10. The status of the network layer service primitives provided by a BCC or DCC is specified as follows:

O: Optional
M: Mandatory
C: Conditional

Table 10— Network layer service requirements

Service primitives	Status	
	BCC	DCC
Device discovery		
LM_DiscoverDevices.request(nr slots)	M	N/A
LM_DiscoverDevices.confirm(status, list of (device address, device info, method))	M	N/A
LM_DiscoverDevices.indication(device address, device info, method)	N/A	M
Connection		
LM_Connect.request(called LSAP, requested QoS, client data)	M	C ^a
LM_Connect.confirm(called LSAP, resultant QoS, client data)	M	C ^a
LM_Connect.indication(calling LSAP, resultant QoS, client data)	C ^a	M
LM_Connect.response(calling LSAP, client data)	C ^a	M
Status		
LM_Status.request()	M	M
LM_Status.indication(link status, lock status)	M	M
LM_Status.confirm(unacked data flag)	M	M
Data transfer		
LM_Data.request(data)	M	M
LM_Data.indication(data)	M	M
LM_UData.request(data)	C ^a	C ^a
LM_UData.indication(data)	C ^a	C ^a
Disconnection		
LM_Disconnect.request(reason, client data)	O ^b	O ^b
LM_Disconnect.indication(reason, client data)	M	M

^aIndicated service is required in a BCC or DCC that supports SNTP.

^bAn IrLAP disconnect may be used in place of an IrLMP disconnect as described in IrDA Lite [B4].

9. Transport layer

The transport layer is adopted from TinyTP, which implements ISO/OSI layer 4, the transport layer. This layer supports multiple transport connections with independent flow control.

TinyTP also defines a capability for data stream segmentation and reassembly (SAR). SAR may be used to achieve a larger maximum transfer unit, if both ends of the link support SAR.

9.1 Maximum transfer unit

The transport profile provides a delivery service for user data. Any client service data unit (SDU) not larger than the maximum transfer unit (MTU) shall be delivered by the transport profile. The MTU is determined according to Table 11. “Data size” is the negotiated IrLAP data size parameter. The MTU is determined independently for each direction of transfer.