



BSI Standards Publication

**Stationary source emissions
— Determination of the
mass concentration of
dinitrogen monoxide (N₂O)
— Reference method: Non-
dispersive infrared method
(ISO 21258:2010)**

National foreword

This British Standard is the UK implementation of EN ISO 21258:2010.

The UK participation in its preparation was entrusted to Technical Committee EH/2/1, Stationary source emission.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© BSI 2010

ISBN 978 0 580 57898 4

ICS 13.040.40

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 July 2010

Amendments issued since publication

Date	Text affected
------	---------------

English Version

Stationary source emissions - Determination of the mass concentration of dinitrogen monoxide (N₂O) - Reference method: Non-dispersive infrared method (ISO 21258:2010)

Émissions de sources fixes - Détermination de la concentration massique de protoxyde d'azote (N₂O) - Méthode de référence: Méthode infrarouge non dispersive (ISO 21258:2010)

Emissionen aus stationären Quellen - Bestimmung der Massenkonzentration von Distickstoffmonoxid (N₂O) - Referenzverfahren: Nicht-dispersives Infrarot-Verfahren (ISO 21258:2010)

This European Standard was approved by CEN on 19 May 2010.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: Avenue Marnix 17, B-1000 Brussels

Foreword

This document (EN ISO 21258:2010) has been prepared by Technical Committee ISO/TC 146 "Air quality" in collaboration with Technical Committee CEN/TC 264 "Air quality" the secretariat of which is held by DIN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by December 2010, and conflicting national standards shall be withdrawn at the latest by December 2010.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and the United Kingdom.

Endorsement notice

The text of ISO 21258:2010 has been approved by CEN as a EN ISO 21258:2010 without any modification.

Contents

Page

Foreword	iv
Introduction.....	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Symbols and abbreviated terms	5
5 Principle.....	6
6 Description of the automated measuring equipment	6
6.1 General	6
6.2 Sampling line components.....	7
6.3 Analyser equipment	8
6.4 Responsibilities	8
7 Performance criteria and determination of the performance characteristics	9
7.1 Performance criteria.....	9
7.2 Determination of the performance characteristics and measurement uncertainty	10
7.3 Establishment of the uncertainty budget.....	10
8 Measurement procedure.....	11
8.1 Sampling location.....	11
8.2 Sampling point(s)	11
8.3 Choice of the measuring system	11
8.4 Setting of the analyser on site	12
9 Ongoing quality control	13
9.1 General	13
9.2 Frequency of checks	13
10 Evaluation of the method in the field	14
11 Expression of results	14
12 Test report.....	15
Annex A (informative) Schematic diagram of a typical analyser	16
Annex B (normative) Procedures for determination of the performance characteristics during the general performance test.....	17
Annex C (informative) Example of assessment of compliance of NDIR method for N ₂ O with requirements on emission measurements	20
Annex D (informative) Results of comparison tests.....	27
Annex E (informative) Leak test procedures	30
Bibliography	32

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 21258 was prepared by Technical Committee ISO/TC 146, *Air quality*, Subcommittee SC 1, *Stationary source emissions*.

Introduction

Dinitrogen monoxide (N_2O , also known as nitrous oxide) is an important greenhouse gas with a global warming potential 310 times that of carbon dioxide (CO_2). N_2O is of both natural and anthropogenic origin. Increased emissions of N_2O have been observed, for example, in the exhaust gas of combustion processes using nitrogenous fuels at temperatures below 900 °C, and in the reduction of NO_x using the selective non-catalytic reduction (SNCR) process, in particular when urea is used. There is considerable uncertainty over current N_2O emissions, which is reflected in the wide range of emission factors cited. The largest uncertainties are for emissions from natural and agricultural sources, which are difficult to measure accurately. In the past, emissions from stationary sources such as coal-fired plants and industry were overestimated due to a serious artefact in the grab-sampling methodology used to measure emissions. N_2O is involved in the EU emission trading scheme along with CO_2 and methane (CH_4).

Improved measurement techniques are helping to reduce uncertainties in emission estimates. Improved measurement techniques are also a prerequisite for accurate information on N_2O and its potential role in the enhanced greenhouse effect.

Stationary source emissions — Determination of the mass concentration of dinitrogen monoxide (N₂O) — Reference method: Non-dispersive infrared method

1 Scope

This International Standard specifies a method for sampling, sample conditioning and determination of dinitrogen monoxide (N₂O) content in the flue gas emitted from ducts and stacks to atmosphere. It sets out the non-dispersive infrared (NDIR) analytical technique, including the sampling system and sample gas conditioning system.

This International Standard is a reference method for periodic monitoring and for calibration, adjustment or control of automatic monitoring systems permanently installed on a stack.

This reference method has been successfully tested on a sewage sludge incinerator where the N₂O concentration in the flue gas was up to about 200 mg/m³.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 9169:2006, *Air quality — Definition and determination of performance characteristics of an automatic measuring system*

ISO 14956, *Air quality — Evaluation of the suitability of a measurement procedure by comparison with a required measurement uncertainty*

ISO/IEC Guide 98-3:2008, *Uncertainty of measurement — Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

influence quantity

quantity that is not the measurand but that affects the result of the measurement

[ISO/IEC Guide 98-3:2008, B.2.10]

3.2

interference

negative or positive effect upon the response of the measuring system, due to a component of the sample that is not the measurand

3.3
interferent
interfering substance

substance present in the air mass under investigation, other than the measurand, that affects the response

[ISO 9169:2006, 2.1.12]

3.4
lack of fit

systematic deviation within the range of application between the measurement results obtained by applying the calibration function to the observed response of the measuring system measuring reference materials and the corresponding accepted value of such reference materials

NOTE 1 Lack of fit may be a function of the measurement result.

[ISO 9169:2006, 2.2.9]

NOTE 2 The expression “lack of fit” is often replaced in everyday language for linear relations by “linearity” or “deviation from linearity”.

3.5
measurand

particular quantity subject to measurement

[ISO/IEC Guide 98-3:2008, B.2.9]

3.6
performance characteristic

one of the quantities assigned to equipment in order to define its performance

NOTE Performance characteristics can be described by values, tolerances, or ranges.

3.7
reference gas

gaseous mixture of stable composition used to calibrate the reference measuring system and which is traceable to national or international standards

3.8
reference method

measurement method taken as a reference by convention, which gives the accepted reference value of the measurand

3.9
repeatability in the laboratory

precision under repeatability conditions in the laboratory

NOTE 1 Repeatability can be expressed quantitatively in terms of the dispersion characteristics of the results. In this International Standard, the repeatability is expressed as a value with a level of confidence of 95 %.

NOTE 2 Adapted from ISO 3534-2:2006^[1], 3.3.5.

3.10
repeatability conditions in the laboratory

observation conditions where independent test results are obtained with the same method on identical test items in the same test or measuring facility by the same operator using the same equipment within short intervals of time in the laboratory

NOTE 1 Repeatability conditions in the laboratory include:

— the same measurement procedure at the same laboratory;

- the same operator;
- the same measuring instrument used under the same conditions;
- the same location;
- repetition over a short period of time.

NOTE 2 Adapted from ISO 3534-2:2006^[1], 3.3.6.

3.11

repeatability in the field

precision under repeatability conditions in the field

NOTE 1 Repeatability can be expressed quantitatively in terms of the dispersion characteristics of the results. In this International Standard the repeatability under field conditions is expressed as a value with a level of confidence of 95 %.

NOTE 2 Adapted from ISO 3534-2:2006^[1], 3.3.5.

3.12

repeatability conditions in the field

observation conditions where independent test results are obtained with the same method on identical test items in the same test or measuring facility by the same operator using the same equipment within short intervals of time in the field

NOTE 1 Repeatability conditions in the field include:

- the same measurement procedure;
- two sets of equipment, the performance of which fulfils the requirements of the reference method, used under the same conditions;
- the same location;
- implemented by the same laboratory;
- typically calculated on short periods of time in order to avoid the effect of changes of influence parameters.

NOTE 2 Adapted from ISO 3534-2:2006^[1], 3.3.6.

3.13

reproducibility in the field

precision under reproducibility conditions in the field

NOTE 1 Reproducibility in the field can be expressed quantitatively in terms of the dispersion characteristics of the results. In this International Standard the reproducibility under field conditions is expressed as a value with a level of confidence of 95 %.

NOTE 2 Adapted from ISO 3534-2:2006^[1], 3.3.10.

NOTE 3 Results are usually understood to be corrected results.

3.14

reproducibility conditions in the field

observation conditions where independent test results are obtained with the same method on identical test items in different test or measurement facilities with different operators using different equipment in the field

NOTE 1 Reproducibility conditions in the field include:

- the same measurement procedure;

- several sets of equipment, the performance of which fulfils the requirements of the reference method, used under the same conditions;
- the same location;
- implemented by several laboratories.

NOTE 2 Adapted from ISO 3534-2:2006^[1], 3.3.11.

3.15

residence time in the measuring system

time period for transportation of the sampled gas from the inlet of the probe to the inlet of the measurement cell

3.16

response time

time interval between the instant when a stimulus is subjected to a specified abrupt change and the instant when the response reaches and remains within specified limits around its final stable value, determined as the sum of the lag time and the rise time in the rising mode, and the sum of the lag time and the fall time in the falling mode

[ISO 9169:2006, 2.2.4]

3.17

span gas

gas or gas mixture used to adjust and check a specific point on the response line of the measuring system

NOTE This concentration is often chosen around 80 % of full scale.

3.18

uncertainty (of measurement)

parameter, associated with the result of a measurement, that characterises the dispersion of the values that could reasonably be attributed to the measurand

[ISO/IEC Guide 98-3:2008, B.2.18]

3.19

standard uncertainty

uncertainty of the result of a measurement expressed as a standard deviation

[ISO/IEC Guide 98-3:2008, 2.3.1]

3.20

combined standard uncertainty

standard uncertainty of the result of a measurement when that result is obtained from the values of a number of other quantities, equal to the positive square root of a sum of terms, the terms being the variances or covariances of these other quantities weighted according to how the measurement result varies with changes in these quantities

[ISO/IEC Guide 98-3:2008, 2.3.4]

3.21

expanded uncertainty

quantity defining an interval around the result of a measurement that may be expected to encompass a large fraction of the distribution of values that could reasonably be attributed to the measurand

[ISO/IEC Guide 98-3:2008, 2.3.5]

NOTE In this International Standard, the expanded uncertainty is calculated with a coverage factor of $k = 2$, and with a level of confidence of 95 %.

3.22

uncertainty budget

list of sources of uncertainty and their associated standard uncertainties, compiled with a view to evaluating a combined standard uncertainty associated with a measurement result

[ISO/TS 21748:2004^[6], 3.13]

3.23

zero gas

gas or gas mixture used to establish the zero point on a calibration curve within a given concentration range

[ISO 12039:2001^[4]]

4 Symbols and abbreviated terms

γ_a	measured concentration of N ₂ O at actual oxygen concentration
γ_d	concentration of N ₂ O on dry basis
γ_n	normalized concentration of N ₂ O
γ_w	measured concentration of N ₂ O on wet basis
$\bar{\gamma}$	grand mean of measured N ₂ O concentration
$\phi_{H_2O,m}$	measured water vapour content, as a percentage volume fraction
$\phi_{O_2,m}$	measured oxygen content, as a volume fraction, in the waste gas
$\phi_{O_2,ref}$	reference oxygen content, as a volume fraction
$C_{V,r}$	coefficient of variation of repeatability
$C_{V,R}$	coefficient of variation of reproducibility
$C_{V,u}$	coefficient of variation of the standard uncertainty
k	coverage factor
n	number of test results
PFA	perfluoroalkoxy
PTFE	polytetrafluoroethylene
QA	quality assurance
QC	quality control
s_j	standard deviation of level j
$s_{r,j}$	repeatability standard deviation
$s_{R,j}$	reproducibility standard deviation
u	standard uncertainty
$u(\gamma_{N_2O})$	combined uncertainty of the measured concentration of N ₂ O
$U(\gamma_{N_2O})$	expanded uncertainty of the measured concentration of N ₂ O


5 Principle

This International Standard describes a reference method for sampling, sample conditioning, and determining N_2O content in the flue gas emitted from ducts and stacks to atmosphere by means of a continuous analyser using non-dispersive infrared method. A number of performance characteristics with associated minimum performance criteria are given for the analyser and details of the uncertainty of the method are presented. Requirements and recommendations for quality assurance and quality control of field measurements are given.

6 Description of the automated measuring equipment

6.1 General

A representative volume of flue gas is extracted from the emission source for a fixed period of time at a controlled flow rate. Dust present in the volume sampled is removed by filtration before the sample is conditioned and passes to the analytical instrument. Figure 1 shows a typical arrangement of a complete measuring system for N_2O .

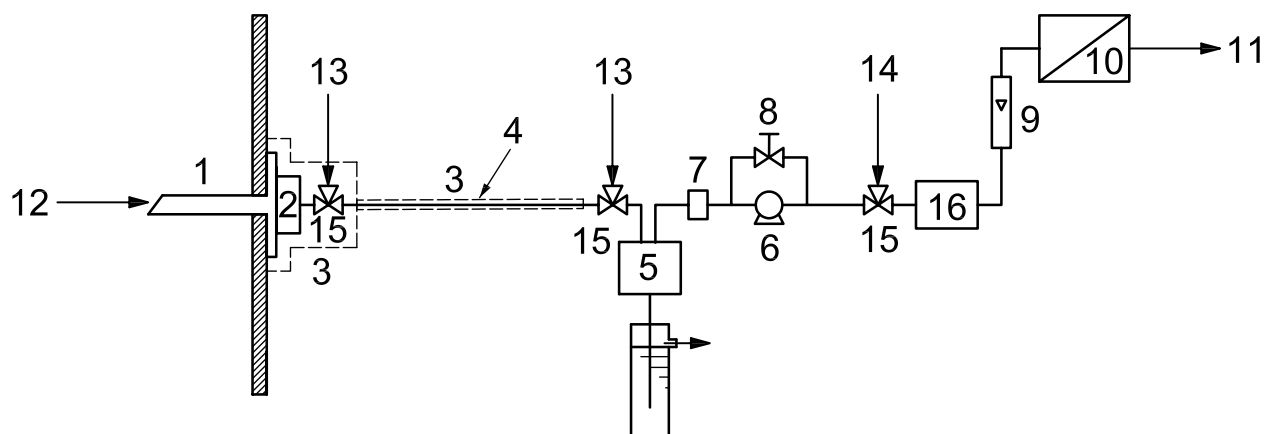

Key

- 1 gas sampling probe
- 2 primary filter
- 3 heating (for use as necessary)
- 4 sampling line (heated as necessary)
- 5 sample cooler with condensate separator
- 6 sample pump
- 7 secondary filter
- 8 needle valve
- 9 flow meter
- 10 N_2O analyser
- 11 output
- 12 inlet for zero and span gas (preferably in front of the nozzle) to check the complete system
- 13 inlet for zero and span gas to check the conditioning system and N_2O analyser
- 14 inlet for zero and span gas to check the converter and N_2O analyser
- 15 valve
- 16 converter for CO oxidation

Figure 1 — Example of the installation of measuring devices