

Stationary source emissions — Determination of PM₁₀/PM_{2,5} mass concentration in flue gas — Measurement at low concentrations by use of impactors (ISO 23210:2009)

ICS 13.040.40

National foreword

This British Standard is the UK implementation of EN ISO 23210:2009.
The UK participation in its preparation was entrusted to Technical Committee EH/2/1, Stationary source emission.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 August 2009
© BSI 2009

ISBN 978 0 580 65743 6

Amendments/corrigenda issued since publication

Date	Comments

English Version

Stationary source emissions - Determination of PM10/PM2,5
mass concentration in flue gas - Measurement at low
concentrations by use of impactors (ISO 23210:2009)

Émissions de sources fixes - Détermination de la
concentration en masse de PM10/PM2,5 dans les effluents
gazeux - Mesurage à des faibles concentrations au moyen
d'impacteurs (ISO 23210:2009)

Emissionen aus stationären Quellen - Ermittlung der
Massenkonzentration von PM10/PM2,5 im Abgas -
Messung bei niedrigen Konzentrationen mit Impaktoren
(ISO 23210:2009)

This European Standard was approved by CEN on 20 June 2009.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: Avenue Marnix 17, B-1000 Brussels

Foreword

This document (EN ISO 23210:2009) has been prepared by Technical Committee ISO/TC 146 "Air quality" in collaboration with Technical Committee CEN/TC 264 "Air quality", the secretariat of which is held by DIN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by February 2010, and conflicting national standards shall be withdrawn at the latest by February 2010.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and the United Kingdom.

Endorsement notice

The text of ISO 23210:2009 has been approved by CEN as a EN ISO 23210:2009 without any modification.

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	2
4 Symbols and abbreviated terms	3
5 Principle of the method	5
6 Specification of the two-stage impactor	8
7 Sampling train	11
8 Preparation, measurement procedure and post-treatment	13
9 Calculation of the results	17
10 Performance characteristics	17
11 Reporting	20
Annex A (normative) Calculation of the sample volumetric flow rate of the impactor	21
Annex B (informative) General equations concerning impaction theory	28
Annex C (informative) Results of method validation	30
Annex D (informative) Influence of variations in the flue gas temperature and flue gas composition on the Reynolds number	36
Annex E (informative) Entry nozzle	38
Annex F (informative) Equipment list	39
Annex G (normative) Determination of a representative sampling point	41
Bibliography	42

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 23210 was prepared by Technical Committee ISO/TC 146, *Air quality*, Subcommittee SC 1, *Stationary source emissions*.

Introduction

In order to quantify the amount of PM₁₀ and PM_{2,5} particles in stationary source emissions or to identify the contribution sources of PM₁₀ and PM_{2,5} in ambient air, it is necessary to measure fine particulate matter in the flue gas of industrial sources.

This International Standard describes a measurement method for the determination of mass concentrations of PM₁₀ and PM_{2,5} emissions, which realizes the same separation curves as those specified in ISO 7708:1995 for PM₁₀ and PM_{2,5} in ambient air. The method is based on the principle of impaction. During sampling, the particle fraction is divided into three groups with aerodynamic diameters greater than 10 µm, between 10 µm and 2,5 µm and smaller than 2,5 µm.

The measurement method allows the simultaneous determination of concentrations of PM₁₀ and PM_{2,5} emissions. The method is designed for stack measurements at stationary emission sources.

The contribution of stationary source emissions to PM₁₀ and PM_{2,5} concentrations in ambient air can be classified as primary and secondary. Those emissions that exist as particulate matter within the stack gas and that are emitted directly to air can be considered “primary”. Secondary particulate consists of those emissions that form in ambient air due to atmospheric chemical reactions. The measurement technique in this International Standard does not measure the contribution of stack emissions to the formation of secondary particulate matter in ambient air.

This International Standard includes normative references to ISO 12141:2002. The corresponding requirements in ISO 12141:2002 are identical to those in European Standards EN 13284-1:2001 and EN 15259:2007.

Stationary source emissions — Determination of PM₁₀/PM_{2,5} mass concentration in flue gas — Measurement at low concentrations by use of impactors

1 Scope

This International Standard specifies a standard reference method for the determination of PM₁₀ and PM_{2,5} mass concentrations at stationary emission sources by use of two-stage impactors. The measurement method is especially suitable for measurements of mass concentrations below 40 mg/m³ as half-hourly averages in standard conditions (273 K, 1 013 hPa, dry gas). It is an acceptable method for the measurement in the flue gas of different installations, such as cement and steel production plants, as well as combustion processes.

This International Standard is not applicable to the sampling of flue gases that are saturated with water vapour.

This International Standard is not applicable where the majority of the particles are likely to exceed PM₁₀, for example, in the case of raw gases or plant operating failures.

NOTE 1 Measurements of particulate concentrations higher than 40 mg/m³, as a half-hourly average in standard conditions (273 K, 1 013 hPa, dry gas), can lead to overloading of the collecting plates and backup filters and also could result in shorter sampling times.

NOTE 2 The collecting plates and backup filters can be used for further chemical analysis.

This International Standard cannot be used for the determination of the total mass concentration of dust.

NOTE 3 For data assessment purposes, it can be useful to perform measurements of total particulate matter in parallel to the PM₁₀ and PM_{2,5} measurements.

This International Standard describes the design, use and theory of round-nozzle impactors. It does not exclude other types of impactors, provided these systems meet the performance criteria specified in this International Standard in a validation of the impactor performed by an independent testing laboratory.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 7708:1995, *Air quality — Particle size fraction definitions for health-related sampling*

ISO 12141:2002, *Stationary source emissions — Determination of mass concentration of particulate matter (dust) at low concentrations — Manual gravimetric method*

ISO 20988:2007, *Air quality — Guidelines for estimating measurement uncertainty*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1 Flow-related terms

3.1.1

aerodynamic diameter

diameter of a sphere of density 1 g/cm^3 with the same terminal velocity due to gravitational force in calm air as the particle, under prevailing conditions of temperature, pressure and relative humidity

NOTE Adapted from ISO 7708:1995, 2.2.

3.1.2

cut-off diameter

aerodynamic diameter where the separation efficiency of the impactor stage is 50 %

3.1.3

PM₁₀

particles which pass through a size-selective inlet with a 50 % efficiency cut-off at $10 \text{ }\mu\text{m}$ aerodynamic diameter

NOTE PM₁₀ corresponds to the “thoracic convention” as defined in ISO 7708:1995, Clause 6.

3.1.4

PM_{2,5}

particles which pass through a size-selective inlet with a 50 % efficiency cut-off at $2,5 \text{ }\mu\text{m}$ aerodynamic diameter

NOTE PM_{2,5} corresponds to the “high-risk respirable convention” as defined in ISO 7708:1995, 7.1.

3.1.5

Reynolds number

dimensionless parameter describing a flow

3.1.6

Stokes's number

dimensionless instrument-specific quantity

NOTE See B.2.

3.1.7

Cunningham factor

correction factor taking into account the change in the interaction between particles and the gas phase

NOTE Stokes's law is based on the assumption that the relative gas velocity at the particle edge equals zero. This assumption is not valid for particle sizes close to the mean free path length. Such particles cannot move continuously due to collisions with particles and gas atoms. In this case, Stokes's law has to be amended by a correction factor, i.e. the Cunningham factor. This factor only depends on the mean free path length and the particle diameter.

3.1.8

Sutherland constant

constant characteristic of a gas used for calculating the dependence of the viscosity of a gas on its temperature

3.1.9

aerosol

suspension in a gaseous medium of solid particles, liquid particles or solid and liquid particles having a negligible falling velocity

[ISO 4225:1994, 3.2]

3.2 Instrument-related terms

3.2.1

filter set

separator consisting of two collecting plates and a backup filter

3.2.2

collecting plate

plane filter used for particle collection by impaction

3.2.3

backup filter

plane filter used for collection of the PM_{2,5} particle fraction

3.2.4

collecting plate holder

support of the collecting plate

3.2.5

backup filter holder

punched plate as support of the backup filter

3.2.6

diffuser

conical part in front of the nozzle plates to avoid stall

3.3 Sampling-related terms

3.3.1

measurement site

sampling site

place on the waste gas duct in the area of the measurement plane(s) consisting of structures and technical equipment

NOTE The measurement site consists, for example, of working platforms, measurement ports and energy supply.

3.3.2

measurement section

region of the waste gas duct which includes the measurement plane(s) and the inlet and outlet sections

3.3.3

measurement plane

sampling plane

plane normal to the centreline of the duct at the sampling position

4 Symbols and abbreviated terms

A separation efficiency

BF backup filter

$c_{1,i}$ i th concentration value of the first measuring system

$c_{2,i}$ i th concentration value of the second measuring system

C Cunningham factor

CP2	collecting plate of the second impactor stage
d_{ae}	aerodynamic diameter
d_e	equivalent volumetric diameter
d_{in}	impactor nozzle diameter
d_{nozzle}	entry nozzle diameter
d_{50}	cut-off diameter
E	collection efficiency
f_n	mass concentration of water vapour in standard conditions and with dry gas
g	acceleration due to gravity
i	series element number, $i = 1, 2, 3, \dots m$
j	series element number, $j = 1, 2, 3, \dots n$
l_{in}	impactor nozzle length
m	sampled mass
$m(BF)$	particle mass on the backup filter
$m(CP2)$	particle mass on the collecting plate of the second impactor stage
M	molar mass
n	number of measurement pairs
N	number of impactor nozzles
p	absolute gas pressure
p_{atm}	atmospheric pressure at the measurement site (barometric pressure)
p_n	standard pressure
p_{st}	difference between the static pressure in the measurement cross-section and the atmospheric pressure at the measurement site
r	volume fraction
R	gas constant
Re	Reynolds number
s	distance between the end of the nozzle and the impactor plate
s_D	standard deviation of paired measurements
S	Sutherland constant
St	Stokes's number

T	gas temperature
T_n	standard temperature
T_{crit}	critical temperature
v_{fg}	flue gas velocity
v_{in}	gas velocity in the impactor nozzle
v_{nozzle}	gas velocity in the entry nozzle
v_p	particle drift rate
V	sample volume
V_n	sample volume in standard conditions and for dry gas
$\dot{V}$	volumetric flow rate
WV	water vapour
λ	mean free path length
χ	dynamic shape factor for non-spherical particles
η	dynamic viscosity of the gas
ρ_n	density of the dry gas in standard conditions
$\rho_{n,\text{WV}}$	density of water vapour in standard conditions
$\rho_{p,t,h}$	density of the gas in operating conditions
ρ_p	particle mass density
$\rho_{0,p}$	particle unit mass density

5 Principle of the method

5.1 General

In particle measurements, the following three relevant physical characteristics can be distinguished:

- mass concentration (e.g. total dust, PM_{10} , $\text{PM}_{2,5}$) and distribution of mass fractions;
- particle number concentration and particle size distribution by number concentration;
- morphology of particles (e.g. shape, colour, optical properties).

The PM_{10} and $\text{PM}_{2,5}$ mass concentrations are determined by size-selective separation of gas-borne particles by use of the different inertia of particles. In general, two methods of separation based on the inertia principle can be distinguished:


- impactors (sub-types: e.g. slot-type nozzle impactor, round-nozzle impactor, virtual impactor);
- cyclones (sub-types: e.g. cascade cyclone, sharp-cut cyclone).

Impactors are used at low mass concentrations, whereas cyclones are applied at high mass concentrations.

This International Standard specifies a measurement method for the determination of PM_{10} and $\text{PM}_{2,5}$ mass concentrations based on impaction with a round-nozzle impactor.

5.2 Theory of impaction

An impactor separates particles according to their specific aerodynamic diameter. The aerosol is accelerated through a nozzle and then deflected by 90°. Particles with greater aerodynamic diameters are not able to follow the gas flow due to their mass inertia. They are impacted on the collecting plate (see Figure 1).

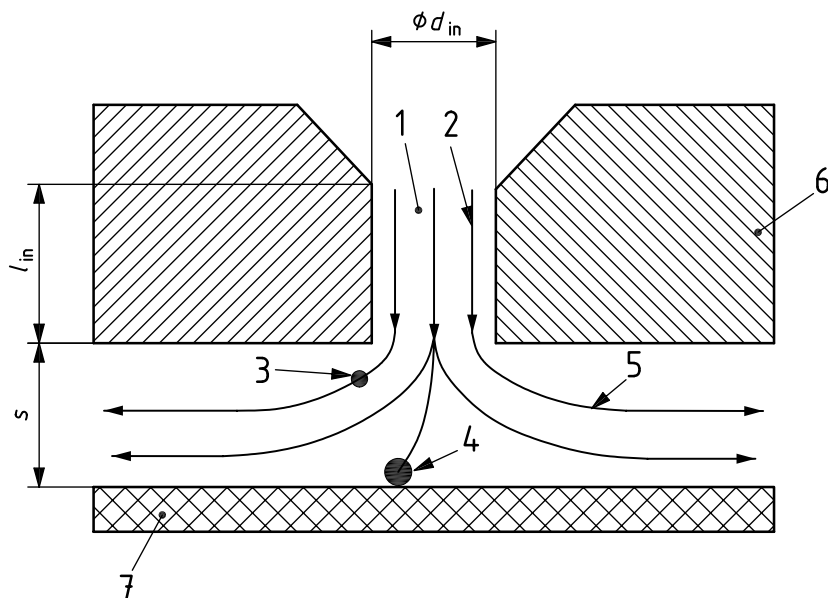

Key

- | | | | |
|---|--------------------------------|----------|---|
| 1 | impactor nozzle | l_{in} | impactor nozzle length |
| 2 | flow line | s | distance between nozzle outlet and collecting plate |
| 3 | particle remaining in the flow | d_{in} | impactor nozzle diameter |
| 4 | impacted particle | | |
| 5 | particle trajectory | | |
| 6 | nozzle plate | | |
| 7 | collecting plate | | |

Figure 1 — Principle of impaction

An impactor stage is defined by the so-called cut-off diameter d_{50} . For particles with this aerodynamic diameter, the separation efficiency of the impactor is 50 %. Equation (1) is used to calculate the cut-off diameter d_{50} of a single-stage round-nozzle impactor (see Reference [11] in the Bibliography):

$$d_{50} = \sqrt{\frac{9\pi St_{50} \eta N d_{in}^3}{4\rho_{0,P} C \dot{V}}} \quad (1)$$

where

St_{50} is the Stokes's number in relation to the cut-off diameter d_{50} ;

η is the dynamic viscosity of the gas;

N is the number of impactor nozzles;

d_{in} is the impactor nozzle diameter;

$\rho_{0,P}$ is the particle unit mass density (1 g/cm³);

C is the Cunningham factor;

$\dot{V}$ is the volumetric flow rate through the impactor in operating conditions.

The following conditions apply to the design and to the application of Equation (1):

a) Distance between nozzle and collecting plate

The ratio of the distance s between the nozzle outlet and the collecting plate to the nozzle diameter d_{in} shall be between

$$0,5 \leq s / d_{in} \leq 5,0 \quad (2)$$

b) Ratio of nozzle length to nozzle diameter

The ratio of the impactor nozzle length l_{in} to the nozzle diameter d_{in} shall be between

$$0,25 \leq l_{in} / d_{in} \leq 2,0 \quad (3)$$

This leads to a uniform flow profile at the nozzle outlet, i.e. the flow has a uniform velocity at the nozzle outlet. If the ratio is too small ($l_{in}/d_{in} < 0,25$), the flow is still non-uniform. If the ratio is too large ($l_{in}/d_{in} > 2,0$), the velocity at the nozzle edge is smaller than the velocity at the centre of the nozzle due to friction.

c) Reynolds number

The Reynolds number Re of the gas flow in the nozzle shall be in the region of laminar flow ($100 < Re < 3\,000$).

5.3 Cut-off diameter

In reality, the particle separation is not ideal. In practice, impactors exhibit separation curves similar to the example shown in Figure 2.

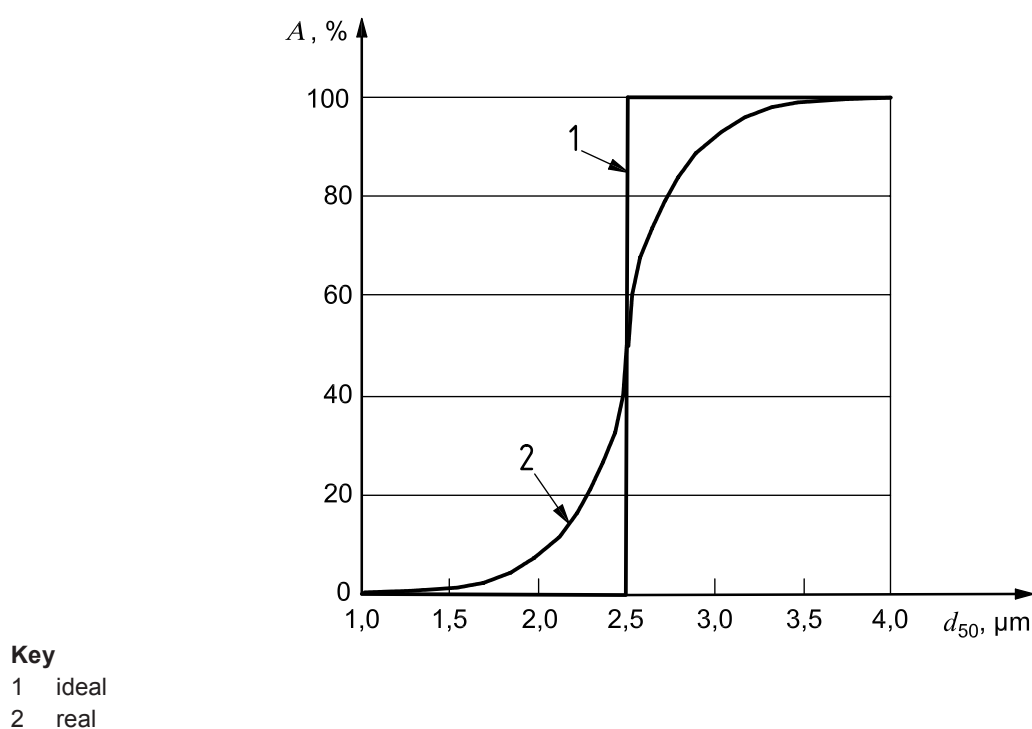


Figure 2 — Separation efficiency A of an impactor as a function of the cut-off diameter d_{50}

5.4 Cascade impactor

This International Standard specifies a two-stage cascade impactor for the determination of PM₁₀ and PM_{2,5} mass concentrations (see Reference [9] in the Bibliography).

NOTE A cascade impactor consists of several impactor stages. The first impactor stage separates the greatest particles on a collecting plate; smaller particles reach the following stages.

The separation curves of PM₁₀ and PM_{2,5} emission measurements shall correspond to the separation curves specified for PM₁₀ and PM_{2,5} ambient air quality measurements. During sampling, the particles are divided into three fractions, with aerodynamic diameters greater than 10 µm, between 10 µm and 2,5 µm, and smaller than 2,5 µm. Therefore, the measurement method allows the simultaneous determination of emission concentrations of PM₁₀ and PM_{2,5}.

6 Specification of the two-stage impactor

6.1 General

The two-stage impactor for the determination of PM₁₀ and PM_{2,5} concentrations in flue gas described in this International Standard divides the particles into the following three fractions:

- a) particles with aerodynamic diameters greater than 10 µm (first impactor stage);
- b) particles with aerodynamic diameters between 10 µm and 2,5 µm (second impactor stage);
- c) particles with aerodynamic diameters smaller than 2,5 µm (backup filter).

The PM_{2,5} mass corresponds to fraction c), and the PM₁₀ mass corresponds to the sum of fractions b) and c). The fraction with aerodynamic diameters greater than 10 µm is not used for the PM₁₀ and PM_{2,5} data evaluation.

6.2 Separation curves

The impactor stages for PM₁₀ and PM_{2,5} shall be designed such that the separation curves of PM₁₀ and PM_{2,5} meet the requirements of the separation efficiencies specified in Tables 1 and 2. The permissible deviations specified in Tables 1 and 2 are absolute percentages concerning the separation efficiencies specified in ISO 7708:1995 (see Figure 3) for the corresponding particle diameters. Furthermore, the requirements of 5.2 shall be fulfilled.

NOTE The shape of the separation curves can differ from the curves shown in Figure 3 due to experimental influences (e.g. detailed design of the impactor and gas flow conditions).

Table 1 — Separation efficiency for the PM_{2,5} impactor stage

Particle diameter	Separation efficiency for mono-disperse latex aerosol and greased collecting plates	Separation efficiency for mono-disperse latex aerosol and quartz-fibre filters
1,0 µm to 2,5 µm ^a	Separation efficiency of ISO 7708:1995 at the corresponding particle diameter with a permissible deviation of ±10 %	Separation efficiency of ISO 7708:1995 at the corresponding particle diameter with a permissible deviation of ±10 %
> 2,5 µm to 10,0 µm ^a	Separation efficiency of ISO 7708:1995 at the corresponding particle diameter with a permissible deviation of ±15 %	Separation efficiency of ISO 7708:1995 at the corresponding particle diameter with a permissible deviation of ±30 %
^a Approximate diameters.		