

Hydraulic fluid power — On-line automatic particle-counting systems for liquids — Methods of calibration and validation

ICS 23.100.01

NO COPYING WITHOUT BSI PERMISSION EXCEPT AS PERMITTED BY COPYRIGHT LAW



Document Sharing Hub

National foreword

This British Standard reproduces verbatim ISO 11943:1999 and implements it as the UK national standard.

The UK participation in its preparation was entrusted to Technical Committee MCE/18, Fluid power systems and components, which has the responsibility to:

- aid enquirers to understand the text;
- present to the responsible international/European committee any enquiries on the interpretation, or proposals for change, and keep the UK interests informed;
- monitor related international and European developments and promulgate them in the UK.

A list of organizations represented on this committee can be obtained on request to its secretary.

Cross-references

The British Standards which implement international or European publications referred to in this document may be found in the BSI Standards Catalogue under the section entitled “International Standards Correspondence Index”, or by using the “Find” facility of the BSI Standards Electronic Catalogue.

A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

Compliance with a British Standard does not of itself confer immunity from legal obligations.

Summary of pages

This document comprises a front cover, an inside front cover, pages i and ii, the ISO title page, pages ii to iv, pages 1 to 28 and a back cover.

This standard has been updated (see copyright date) and may have had amendments incorporated. This will be indicated in the amendment table on the inside front cover.

This British Standard, having been prepared under the direction of the Engineering Sector Committee, was published under the authority of the Standards Committee and comes into effect on 15 October 1999

© BSI 04-2000

ISBN 0 580 32978 X

Amendments issued since publication

Amd. No.	Date	Comments

Contents

	Page
National foreword	Inside front cover
Foreword	iv
Text of ISO 11943	1

INTERNATIONAL STANDARD

**ISO
11943**

First edition
1999-08-01

Hydraulic fluid power — On-line automatic particle-counting systems for liquids — Methods of calibration and validation

*Transmissions hydrauliques — Systèmes de comptage automatique
en ligne de particules en suspension dans les liquides — Méthode
d'étalonnage et de validation*



Contents

	Page
Foreword	iv
Introduction	1
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Units of measurements	1
5 Prerequisite	1
6 Test equipment	1
7 Accuracy of measuring equipment and test conditions	2
8 Off-line calibration procedure	2
9 Validation of on-line sample preparation equipment and determination of secondary calibration standard	2
10 On-line secondary calibration and verification procedure	5
11 On-line dilution system validation	9
12 Precautions	11
13 Identification statement	12
Annex A (informative) Typical on-line calibration and validation system design information guide	13
Annex B (informative) Hydraulic circuit design information guide for on-line counter adaptation to a Multi-pass test stand	15
Annex C (informative) Summary of ISO round robin study for on-line calibration and validation	19
Figure 1 — Flowchart for the validation procedure of on-line sample preparation equipment and determination of secondary calibration standard	3
Figure 2 — Flowchart of procedure for on-line calibration verification	7
Figure 3 — Flowchart of the procedure for on-line dilution system validation	10
Figure A.1 — Example of a system for on-line calibration and validation	14
Figure B.1 — Example of the circuit number 1 for an on-line counter adaptation to the Multi-pass test stand	16
Figure B.2 — Example of the hydraulic circuit number 2 for on-line counter adaptation to Multi-pass test stand	17
Figure B.3 — Example of the hydraulic circuit number 3 for on-line counter adaptation to Multi-pass test stand	18
Figure C.1 — Standard deviation in relation to count from the secondary calibration	20
Table 1 — Measuring equipment accuracy and test conditions	2
Table 2 — Secondary calibration dust data sheet	4
Table 3 — Particle counts for ISO MTD	6
Table 4 — Data sheet for calibration verification	9
Table 5 — Data sheet for validation of on-line dilution equipment	12
Table C.1 — Original ACFTD calibration data	21
Table C.2 — Data after recalibration with ACFTD	22
Table C.3 — Secondary calibration data — Mean counts	23
Table C.4 — Secondary calibration data — Standard deviations	24
Table C.5 — Particle counts for ISO MTD	25
Table C.6 — On-line calibration verification	26

	Page
Table C.7 — On-line dilution validation for upstream sensor	27
Table C.8 — On-line dilution validation for downstream sensor	28

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 3.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 11943 was prepared by Technical committee ISO/TC 131, *Fluid power systems*, Subcommittee SC 6, *Contamination control and hydraulic fluids*.

Annex A, Annex B and Annex C of this International Standard are for information only.

Introduction

In hydraulic fluid power systems, power is transmitted and controlled through a fluid under pressure within an enclosed circuit. The fluid is both a lubricant and a power-transmitting medium.

Reliable system performance requires control of the fluid medium. Qualitative and quantitative determination of particulate contaminant in the fluid medium requires precision in obtaining the sample and determining the size and distribution of the contamination.

Automatic particle counters are an accepted means for determining the size and distribution of particulate contamination in fluids. Individual instrument accuracy is established through calibration.

Automatic particle counters are being utilized on-line to eliminate the need for sample containers, to provide increased accuracy, and to provide for a more rapid access to particle count information. This International Standard establishes guidelines for calibration and validation of on-line automatic particle counters.

1 Scope

This International Standard establishes a calibration and validation process for the use of on-line, automatic particle counting of suspended particles in liquids. A primary use is in the Multi-pass filter test ISO 16889.

2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this International Standard. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 1000:1992, *SI units and recommendations for the use of their multiples and of certain other units*.

ISO 1219-1:1991, *Fluid power systems and components — Graphic symbols and circuit diagrams — Part 1: Graphic symbols*.

ISO 4021:1992, *Hydraulic fluid power — Particulate contamination analysis — Extraction of fluid samples from lines of an operating system*.

ISO 5598:1985, *Fluid power systems and components — Vocabulary*.

ISO 11171:—, *Hydraulic fluid power — Calibration of automatic particle counters for liquids*¹⁾.

ISO 12103-1:1997, *Road vehicles — Test dust for filter evaluation — Part 1: Arizona test dust*.

ISO 16889:—, *Hydraulic fluid power — Filters — Multi-pass method for evaluating filtration performance of a filter element*²⁾.

3 Terms and definitions

For terms and definitions of terms, see ISO 5598.

4 Units of measurements

The international system of units (SI) is used in accordance with ISO 1000.

Throughout this International Standard, the use of $\mu\text{m}(\text{c})$ means that particle size measurements are carried out using an automatic particle counter which has been calibrated in accordance with ISO 11171.

5 Prerequisite

It is assumed that users of this procedure are competent in the operation of their particular particle counter and filter test equipment. It is also important that proper sample handling techniques be utilized throughout the procedure.

6 Test equipment

6.1 Automatic particle counter(s) or particle counter with two independent sensors for liquids.

6.2 Calibration supplies, in accordance with ISO 11171.

6.3 ISO medium test dust (ISO MTD) in accordance with ISO 12103-1, category A3, dried at 110 °C to 150 °C for at least 1 h and for use in the test system, mixed in the test fluid, mechanically agitated, then dispersed ultrasonically with a power density of 3 000 W/m² to 10 000 W/m².

NOTE This standard test dust is used in ISO 16889 for filter test purposes. For availability of ISO MTD, contact the ISO secretariat service or national members of ISO.

¹⁾ To be published. (Revision of ISO 4402:1991)

²⁾ To be published. (Revision of ISO 4572:1981)

6.4 Test fluid, as specified in ISO 16889.

6.5 On-line sample preparation equipment, for mixing and supplying secondary calibration and validation fluid, comprising

- a) a reservoir, pump, fluid conditioning apparatus and instrumentation which are capable of meeting the validation requirements of clause 9;
- b) a clean-up filter capable of providing an initial fluid contamination level less than 5 particles greater than 5 μm (c) per millilitre;
- c) a configuration which will not alter the contaminant distribution over the anticipated test duration (refer to ISO 16889);
- d) fluid sampling sections in accordance with ISO 4021;
- e) a configuration which will supply contaminated fluid to the particle counters under constant flow and temperature within the limits of Table 1.

NOTE 1 A Multi-pass test rig (see ISO 16889) can be used provided it has been validated per clause 9 of this procedure.

NOTE 2 An alternative typical configuration which has proved to be satisfactory is given in Annex A.

6.6 Hydraulic circuit, containing dilution equipment, if required, for on-line counter adaptation to the Multi-pass test stand.

For typical hydraulic circuit configurations which have proven to be satisfactory refer to Annex B.

7 Accuracy of measuring equipment and test conditions

7.1 Utilize measuring equipment with an accuracy within the limits in Table 1.

8 Off-line calibration procedure

8.1 Conduct a sizing calibration on particle counters when new or after major service as suggested by the particle counter manufacturer or in accordance with ISO 11171.

8.2 Use the procedures specified in ISO 11171 to determine particle concentration limits of each particle counter and sensor or use the manufacturer's recommended levels obtained in a similar manner.

9 Validation of on-line sample preparation equipment and determination of secondary calibration standard (see Figure 1)

9.1 When two counters (sensors) are to be used, the procedure described in this clause need only be performed using one counter and sensor.

9.2 Use one particle counter and sensor calibrated in accordance with 8.1 and set to the cumulative mode and at least six different threshold settings over the particle size range of interest.

9.3 Adjust total fluid volume, expressed in litres, in sample preparation equipment to the desired level and measure within $\pm 1\%$. Maintain fluid viscosity at $(15 \pm 0,3) \text{ mm}^2/\text{s}$.

9.4 Use a clean-up filter to provide an initial fluid contamination level less than 5 particles greater than 5 μm (c) per millilitre.

9.5 Determine the contaminant concentration to be used for calibration and verification. The dust concentration should produce a maximum particle count at the lowest particle size of approximately 50 % of the particle counter concentration limit determined in 8.2.

9.6 Add the required quantity of ISO MTD, prepared in accordance with 6.3, to the reservoir and allow to circulate for approximately 15 min. Record the lot number of the ISO MTD.

9.7 Start the test by conducting on-line automatic particle counts (sample volumes of 25 ml are recommended) at 2 min intervals for 1 h or 30 intervals spaced evenly throughout the longest period of time that the system will be used.

Table 1 — Measuring equipment accuracy and test conditions

Test condition	SI Unit	Instrument accuracy ($\pm$ of reading)	Allowed test condition variation
Flow	l/min	0,5 %	2 %
Kinematic viscosity	mm^2/s	1 %	2 %
Pressure	Pa (bar)	1 %	2 %
Temperature	$^{\circ}\text{C}$	0,5 $^{\circ}\text{C}$	1 $^{\circ}\text{C}$
Time	s	0,05 s	0,1 s
Volume	l	0,5 %	1 %
Mass	g	0,1 mg	1 %

CAUTION — Maintaining the accuracy of test conditions to within the limits of Table 1 does not imply that by so doing the validation limits will be satisfied. It has been proven that the most useful way in attaining the validation requirements is by maintaining the accuracy of test conditions given in Table 1 along with using the proper particle counting procedures, etc.

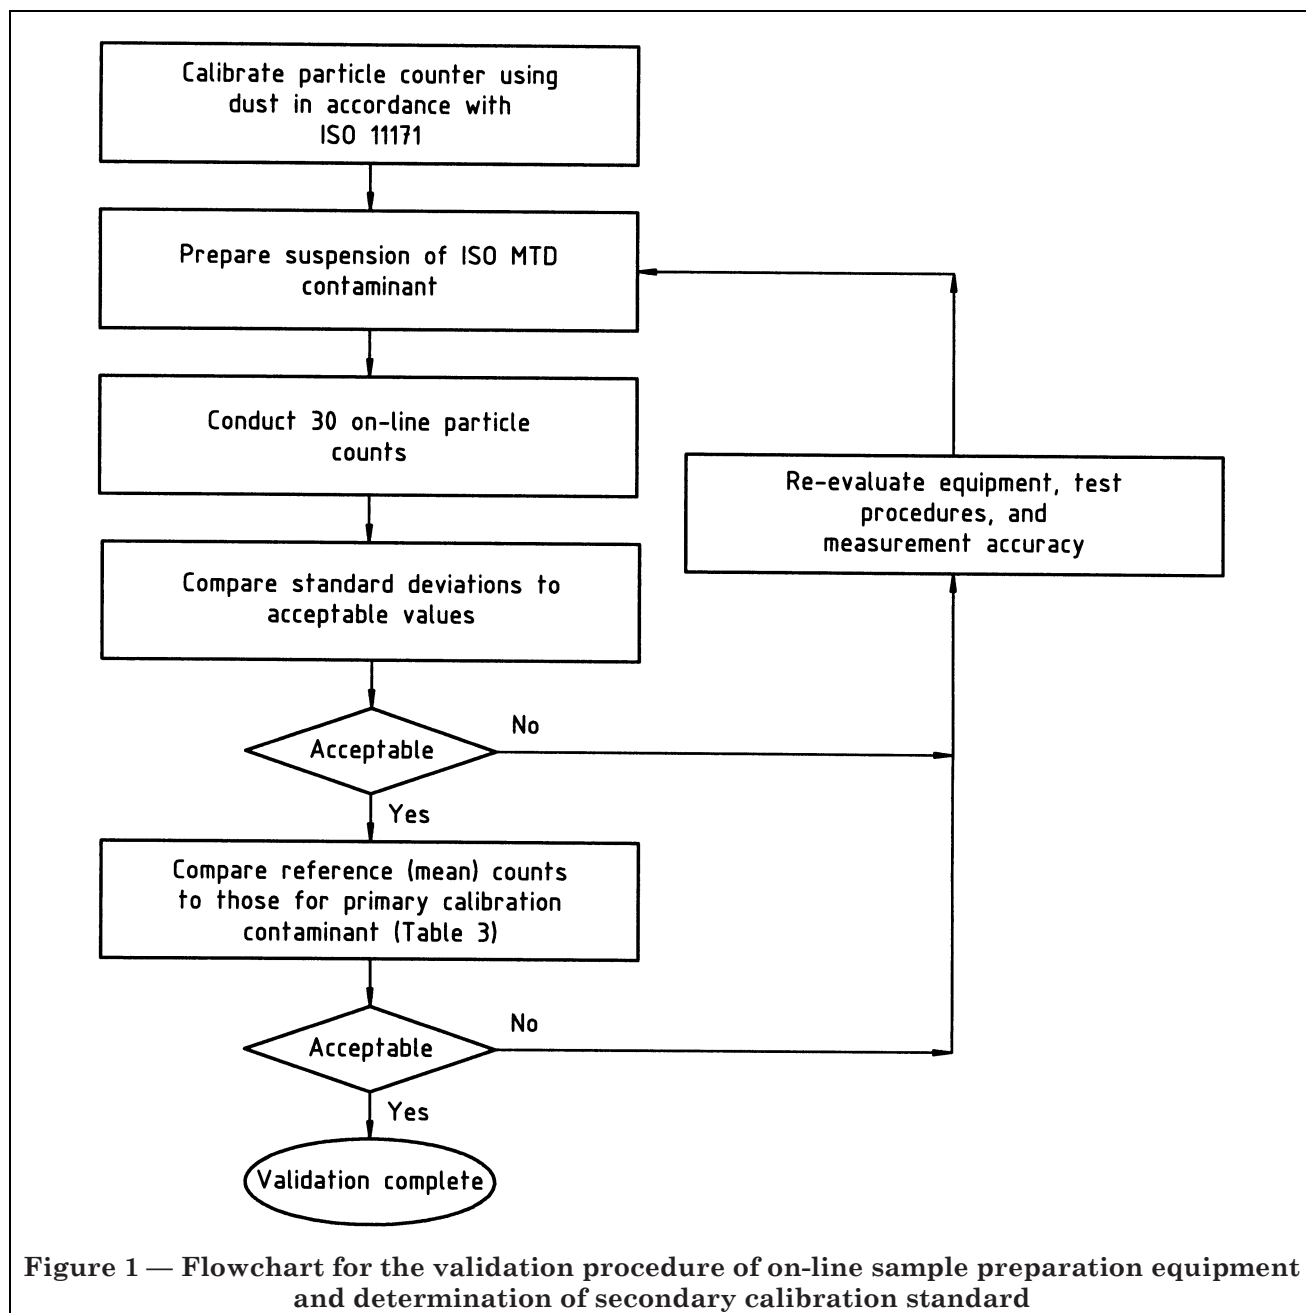


Figure 1 — Flowchart for the validation procedure of on-line sample preparation equipment and determination of secondary calibration standard

Table 2 — Secondary calibration dust data sheet

ISO MTD lot no.: _____ Concentration: _____ mg/l Particle count volume: _____ ml

Operator: _____ Date: _____ Particle counter model: _____

Particle counter serial no.: _____ Sensor model: _____

Sensor serial no.: _____ ISO 11171 primary calibration date: _____

	Number of particles						
Size, $\mu\text{m(c)} >$							
Count 1							
Count 2							
Count 3							
Count 4							
Count 5							
Count 6							
Count 7							
Count 8							
Count 9							
Count 10							
Count 11							
Count 12							
Count 13							
Count 14							
Count 15							
Count 16							
Count 17							
Count 18							
Count 19							
Count 20							
Count 21							
Count 22							
Count 23							
Count 24							
Count 25							
Count 26							
Count 27							
Count 28							
Count 29							
Count 30							
Mean							
σ							
Acceptable σ							