BS ISO 16063-31:2009+A1:2025

BSI Standards Publication

Methods for the calibration of vibration and shock transducers

Part 31: Testing of transverse vibration sensitivity

Documents
Document Sharing Hub

Full document details: BS ISO 16063-31:2009+A1:2025

National foreword

This British Standard is the UK implementation of ISO 16063-31:2009+A1:2025. It supersedes BS ISO 16063-31:2009, which is withdrawn.

The start and finish of text introduced or altered by amendment is indicated in the text by tags. Tags indicating changes to ISO text carry the number of the ISO amendment. For example, text altered by ISO amendment 1 is indicated by A1 A1.

The UK participation in its preparation was entrusted to Technical Committee GME/21, Mechanical vibration, shock and condition monitoring.

A list of organizations represented on this committee can be obtained on request to its committee manager.

Contractual and legal considerations

This publication has been prepared in good faith, however no representation, warranty, assurance or undertaking (express or implied) is or will be made, and no responsibility or liability is or will be accepted by BSI in relation to the adequacy, accuracy, completeness or reasonableness of this publication. All and any such responsibility and liability is expressly disclaimed to the full extent permitted by the law.

This publication is provided as is, and is to be used at the recipient's own risk.

The recipient is advised to consider seeking professional guidance with respect to its use of this publication.

This publication is not intended to constitute a contract. Users are responsible for its correct application.

© The British Standards Institution 2025
Published by BSI Standards Limited 2025

ISBN 978 0 539 27338 0

ICS 17.160

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 30 November 2009.

Amendments/corrigenda issued since publication

Date	Text affected
31 March 2025	Implementation of ISO amendment 1:2025

AVA Documents
Document Sharing Hub

Full document details: BS ISO 16063-31:2009+A1:2025

INTERNATIONAL STANDARD

ISO 16063-31 +A1

First edition
2009-08-15

Amendment 1
2025-03

Methods for the calibration of vibration and shock transducers —

Part 31: Testing of transverse vibration sensitivity

Méthodes pour l'étalonnage des transducteurs de vibrations et de chocs —

Partie 31: Essai de sensibilité aux vibrations transversales

Reference number
ISO 16063-31:2009(E)

Documents
Document Sharing Hub
© ISO 2009

Full document details: BS ISO 16063-31:2009+A1:2025

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

COPYRIGHT PROTECTED DOCUMENT

© ISO 2009

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Documents
Document Sharing Hub

© ISO 2009 – All rights reserved

Full document details: BS ISO 16063-31:2009+A1:2025

Contents

Page

Foreword iv

1 Scope 1

2 Normative references 1

3 Uncertainty considerations 2

4 Determination of transverse sensitivity using a single-axis vibration generator 2
4.1 Apparatus 2
4.2 Method 2
4.2.1 Test procedure 2
4.2.2 Expression of results 3

5 Determination of the transverse sensitivity using a vibration generator with turntable 4
5.1 Apparatus 4
5.2 Method 6
5.3 Expression of results 6

6 Determination of transverse sensitivity using a test system with X- and Y-vibration generators 6
6.1 Apparatus 6
6.2 Method and expression of results 9

7 Determination of the transverse sensitivity using a tri-axial vibration generator 11
7.1 Apparatus 11
7.2 Method and expression of results 14
A1 7.3 Determination of the transverse sensitivity using elliptical orbits 14 A1

8 Equipment for measuring of the input and output signals of the transducer to be tested 15

9 Preferred amplitudes and frequencies 15

Annex A (normative) Definition of transverse sensitivity 16

A1 Annex B (normative) Testing of transverse sensitivity using elliptical orbits 18 A1

Bibliography 20

© ISO 2009 – All rights reserved

Documents
Document Sharing Hub

Full document details: BS ISO 16063-31:2009+A1:2025

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 16063-31 was prepared by Technical Committee ISO/TC 108, *Mechanical vibration, shock and condition monitoring*, Subcommittee SC 3, *Use and calibration of vibration and shock measuring instruments*.

This first edition cancels and replaces ISO 5347-11:1993.

ISO 16063 consists of the following parts, under the general title *Methods for the calibration of vibration and shock transducers*:

— *Part 1: Basic concepts*

— *Part 11: Primary vibration calibration by laser interferometry*

— *Part 12: Primary vibration calibration by the reciprocity method*

— *Part 13: Primary shock calibration using laser interferometry*

— *Part 15: Primary angular vibration calibration by laser interferometry*

— *Part 21: Vibration calibration by comparison to a reference transducer*

— *Part 22: Shock calibration by comparison to a reference transducer*

— *Part 31: Testing of transverse vibration sensitivity*

— *Part 41: Calibration of laser vibrometers*

The following parts are planned:

— Part 23: Angular vibration calibration by comparison to reference transducers

— Part 32: Resonance testing[1)]

— Part 42: Calibration of seismometers

1) Revision of ISO 5347-14:1993 and ISO 5347-22:1997.

© ISO 2009 – All rights reserved
Documents
Document Sharing Hub
Full document details: BS ISO 16063-31:2009+A1:2025

Methods for the calibration of vibration and shock transducers —

Part 31: Testing of transverse vibration sensitivity

1 Scope

This part of ISO 16063 specifies details of the instrumentation and methods to be used for transverse vibration sensitivity testing. It applies to rectilinear velocity and acceleration transducers.

The methods and procedures specified in this part of ISO 16063 allow the determination of the sensitivity of a transducer to vibration in the plane perpendicular to its geometric axis of sensitivity (see Annex A). Because the magnitude of this transverse sensitivity can vary with the direction of the applied vibration, the various methods determine the maximum value. Using that value, the ratio of the transverse sensitivity to the sensitivity on the geometric axis of the transducer can be calculated. In addition, the angle at which the maximum transverse sensitivity occurs can be determined.

The methods and techniques specified can be applied without re-mounting the transducer away from its mounting surface during the test, thus avoiding significant uncertainties often encountered in methods which require repeated mounting. The different methods specified use a single-axis vibration exciter, a two-axis vibration exciter or a tri-axial vibration exciter. Tri-axial vibration excitation allows the transverse sensitivity and the sensitivity on the geometric axis to be determined simultaneously, thus simulating application conditions where the transducer is exposed to multi-axial vibration.

NOTE In accelerometer designs using a bending beam, the transverse sensitivity measured without any vibration acting on the geometric axis of sensitivity of the accelerometer may considerably differ from the transverse sensitivity measured in the presence of a vibration acting on the geometric axis of sensitivity (i.e. when the bending beam is deflected by a vibration to be measured).

This part of ISO 16063 is applicable to a frequency range from 1 Hz to 5 kHz and for a dynamic range from 1 m/s^2 to 1 000 m/s^2 (frequency dependent) and from 1 mm/s to 1 m/s (frequency dependent). Although among all the systems specified it is possible to achieve these ranges, generally each has limitations permitting its use in much smaller ranges.

The methods specified are by comparison both to a reference transducer and to a laser interferometer.

The methods specified allow an expanded uncertainty of the transverse sensitivity (coverage factor k = 2) of 0,1 % or less to be achieved, if the expanded uncertainty is expressed as a percentage of the sensitivity of the test transducer in its sensitive axis.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 266, *Acoustics — Preferred frequencies*

ISO 16063-1:1998, *Methods for the calibration of vibration and shock transducers: Part 1: Basic concepts*

Documents
Document Sharing Hub

© ISO 2009 – All rights reserved

Full document details: BS ISO 16063-31:2009+A1:2025

3 Uncertainty considerations

An expanded uncertainty of 0,1 % (see Clause 1) means, for the example of a transverse sensitivity of 1 %, that the measured value lies within the interval of 0,9 % to 1,1 %.

All users of this part of ISO 16063 are expected to assess and report the uncertainty of measurement according to ISO 16063-1:1998, Annex A, to document their uncertainty expressed as expanded uncertainties for a coverage factor of 2 or a coverage probability of 95 %. It is the responsibility of the laboratory or end user to make sure that the reported values of expanded uncertainty are credible.

4 Determination of transverse sensitivity using a single-axis vibration generator

4.1 Apparatus

The single-axis test system of transverse sensitivity specified in this clause consists of a single-axis vibration exciter that is equipped with a specially designed fixture that enables the transducer under test to be mounted such that its geometric axis of sensitivity is perpendicular to the direction of motion of the vibration exciter table (where the direction of the motion of the vibration exciter table shown in Figure 1 is defined as the Z-direction). It shall be possible to mount the test transducer at different angles about its sensitive axis, preferably for continuous rotation over at least 180°. An example (Reference [5]) of an octahedral fixture is shown in Figure 1.

Another example is the use of an electro-dynamic long-stroke vibration exciter operated in combination with a turntable driven by a stepper motor as specified in Clause 5. The amplitude of the transverse acceleration of the fixture due to transverse motion inherent in the vibration exciter shall be less than 1 % of the acceleration amplitude in the Z-direction at each of the test frequencies. For cases in which the measured transverse sensitivity is less than 2 % of the sensitivity measured on the geometric axis, the transverse motion of the vibration exciter shall meet even higher requirements (e.g. 0,2 % at the test frequencies). To ensure that the transverse motion of the vibration exciter is sufficiently small, measurements of the transverse motion of the total setup (vibration exciter with fixture) with a load close in shape and weight to the transducer being tested should be performed beforehand or the transverse motion could be monitored during the measurement of the transverse sensitivity. For the measurement of the input and output signal of the transducer to be tested, see Clause 8.

The frequency range of the transverse test system is generally 1 Hz to 5 kHz, depending on the working range of the vibration exciter, and on the mass of the fixtures and of the transducer tested. Acceleration amplitudes from 1 m/s^2 to 200 m/s^2 can be generated.

4.2 Method

4.2.1 Test procedure

Vibrate the transducer at the reference amplitude and frequency on the geometric axis of sensitivity to determine its sensitivity, S_N (briefly referred to as S). Determine the values of transverse sensitivity as a function of frequency, S_T, by vibrating perpendicularly to the sensitive axis of the transducer at different angles about its sensitive axis.

The directions and magnitudes of the maximum and minimum transverse sensitivity shall be reported at a designated test frequency or as a function of frequency.

© ISO 2009 – All rights reserved
Documents
Document Sharing Hub
Full document details: BS ISO 16063-31:2009+A1:2025

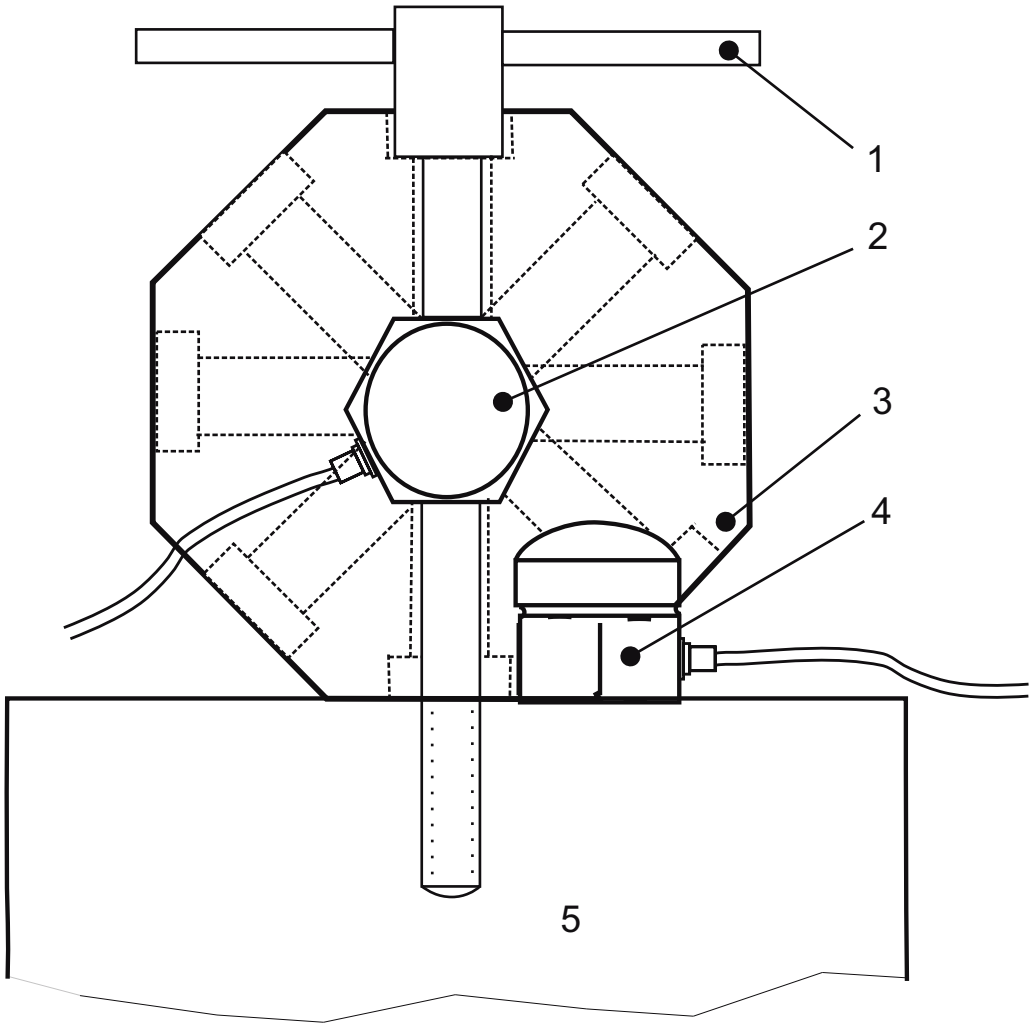

Key

1 screw unit for re-mounting the octahedron in different positions (angle shifts of 45°)
2 transducer to be tested
3 octahedron
4 reference accelerometer
5 vibration exciter table

Figure 1 — Example of a fixture for mounting the test transducer with its sensitive axis perpendicular to the direction of the vibration generated by the vibration exciter

4.2.2 Expression of results

Calculate the transverse sensitivity, S_T, using Equation (1):

$$S_T = \frac{\hat{u}_{out}}{\hat{a}_T} \tag{1}$$

where

$\hat{u}_{out}$ is the amplitude of the output signal of the transducer vibrating perpendicularly to its sensitive axis;

$\hat{a}_T$ is the amplitude of the acceleration in the test direction.

© ISO 2009 – All rights reserved

Documents
Document Sharing Hub
Full document details: BS ISO 16063-31:2009+A1:2025