

Rubber — Calibration and verification of hardness testers

ICS 83.060

National foreword

This British Standard was published by BSI. It is the UK implementation of ISO 18898:2006.

The UK participation in its preparation was entrusted to Technical Committee PRI/20, Accuracy of rubber and plastics test equipment.

A list of organizations represented on PRI/20 can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 30 November 2006

© BSI 2006

ISBN 0 580 49765 8

Amendments issued since publication

Amd. No.	Date	Comments

INTERNATIONAL STANDARD

ISO
18898

First edition
2006-10-01

Rubber — Calibration and verification of hardness testers

Caoutchouc — Étalonnage et vérification des duromètres



Reference number
ISO 18898:2006(E)



Documents

Document Sharing Hub

Contents

Page

Foreword.....	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions.....	1
4 Measurands and metrological requirements for calibration and verification	1
4.1 Environmental conditions.....	1
4.2 Metrological requirements.....	1
5 Calibration and verification methods	8
5.1 Requirements to be met by the measuring instruments used for the calibration and verification methods.....	8
5.2 Outline of the calibration and verification methods to be used	9
5.2.1 Indentors.....	9
5.2.2 Geometry of the pressure foot	9
5.2.3 Depth of indentation	9
5.2.4 Contact force of the pressure foot.....	14
5.2.5 Spring force.....	14
5.2.6 Contact and total force of IRHD dead-load instruments.....	17
5.2.7 Duration of force application.....	18
6 Calibration and verification certificate	18

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 18898 was prepared by Technical Committee ISO/TC 45, *Rubber and rubber products*, Subcommittee SC 2, *Testing and analysis*.

Rubber — Calibration and verification of hardness testers

1 Scope

This International Standard specifies procedures for the calibration and verification of durometers of types A, D, AO and AM (see ISO 7619-1), IRHD pocket meters (see ISO 7619-2) and IRHD dead-load instruments (see ISO 48).

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 48, *Rubber, vulcanized or thermoplastic — Determination of hardness (hardness between 10 IRHD and 100 IRHD)*

ISO 7619-1, *Rubber, vulcanized or thermoplastic — Determination of indentation hardness — Part 1: Durometer method (Shore hardness)*

ISO 7619-2, *Rubber, vulcanized or thermoplastic — Determination of indentation hardness — Part 2: IRHD pocket meter method*

ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories*

ISO 18899, *Rubber — Guide to the calibration of test equipment*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 48 and ISO 18899 apply.

4 Measurands and metrological requirements for calibration and verification

4.1 Environmental conditions

The ambient temperature of the measurement room in which the calibration or verification is carried out shall be 18 °C to 25 °C.

4.2 Metrological requirements

The measurands of indenter and pressure foot for the instrument to be calibrated are depicted in Figures 1 to 6 and requirements are specified in Tables 1 to 9.

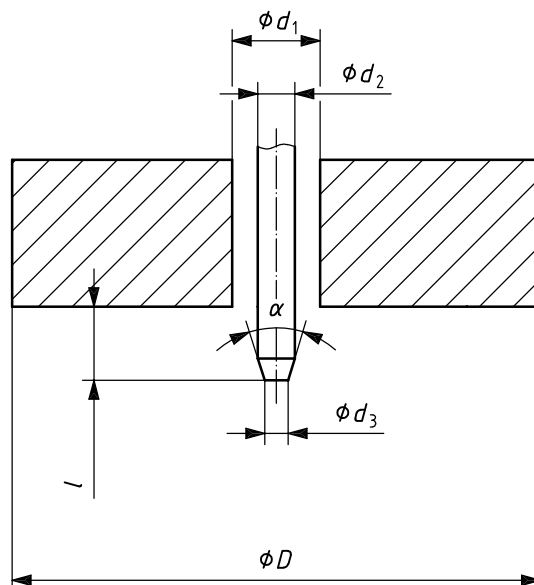


Figure 1 — Indentor and pressure foot for type A durometer

Table 1 — Type A durometer

Measurand	Unit	Metrological requirement	Calibration and verification instructions
Shaft diameter of indentor d_2	mm	$1,25 \pm 0,15$	5.2.1.2
Cone frustum top diameter d_3	mm	$0,79 \pm 0,01$	5.2.1.2
Cone angle of indentor α	°	$35 \pm 0,25$	5.2.1.2
Centrality of pressure foot		Central	
Diameter of pressure foot D	mm	$18 \pm 0,5$	5.2.2.1
Hole diameter of pressure foot d_1	mm	$3 \pm 0,1$	5.2.2.2
Mass on pressure foot m	kg	$1^{+0,1}_0$	5.2.4.1
Depth of indentation l	mm	$0,0$ to $2,50$; $\Delta l = \pm 0,02$	5.2.3.1
Spring force on indentor F	mN	$F = 550 + 75H_A$; $\Delta F = \pm 37,5$ where H_A = hardness reading on type A durometer	5.2.5.1
Duration of force application t	s	3 or 15	5.2.7