

INTERNATIONAL STANDARD



**Explosive atmospheres –
Part 29-2: Gas detectors – Selection, installation, use and maintenance of
detectors for flammable gases and oxygen**



THIS PUBLICATION IS COPYRIGHT PROTECTED

Copyright © 2015 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester. If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

IEC Central Office
3, rue de Varembe
CH-1211 Geneva 20
Switzerland

Tel.: +41 22 919 02 11
info@iec.ch
www.iec.ch

About the IEC

The International Electrotechnical Commission (IEC) is the leading global organization that prepares and publishes International Standards for all electrical, electronic and related technologies.

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigenda or an amendment might have been published.

IEC Catalogue - webstore.iec.ch/catalogue

The stand-alone application for consulting the entire bibliographical information on IEC International Standards, Technical Specifications, Technical Reports and other documents. Available for PC, Mac OS, Android Tablets and iPad.

IEC publications search - webstore.iec.ch/advsearchform

The advanced search enables to find IEC publications by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, replaced and withdrawn publications.

IEC Just Published - webstore.iec.ch/justpublished

Stay up to date on all new IEC publications. Just Published details all new publications released. Available online and also once a month by email.

Electropedia - www.electropedia.org

The world's leading online dictionary of electronic and electrical terms containing 21 000 terms and definitions in English and French, with equivalent terms in 16 additional languages. Also known as the International Electrotechnical Vocabulary (IEV) online.

IEC Glossary - std.iec.ch/glossary

67 000 electrotechnical terminology entries in English and French extracted from the Terms and Definitions clause of IEC publications issued since 2002. Some entries have been collected from earlier publications of IEC TC 37, 77, 86 and CISPR.

IEC Customer Service Centre - webstore.iec.ch/csc

If you wish to give us your feedback on this publication or need further assistance, please contact the Customer Service Centre: sales@iec.ch.



IEC 60079-29-2

Edition 2.0 2015-03
REDLINE VERSION

INTERNATIONAL STANDARD



**Explosive atmospheres –
Part 29-2: Gas detectors – Selection, installation, use and maintenance of
detectors for flammable gases and oxygen**

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

ICS 29.260.20

ISBN 978-2-8322-2455-7

Warning! Make sure that you obtained this publication from an authorized distributor.

CONTENTS

FOREWORD.....	8
INTRODUCTION.....	11
1 Scope.....	13
2 Normative references	14
3 Terms and definitions	15
3.1 Gas properties and other physics.....	15
3.2 Types of equipment	17
3.3 Sensors and detectors	18
3.4 Supply of gas to instruments	20
3.5 Signals and alarms	20
3.6 Times, checks and equipment behaviour.....	21
3.7 Terms exclusive to open path equipment	22
4 Basic information on the properties, behaviour, ~~and detection of~~ gases and vapours, ~~and specific applications of gas detection~~	24
4.1 Detecting gases and vapours ~~—General~~	24
4.1.1 General	24
4.1.2 Safety when monitoring for flammable gases where personnel could be present	25
4.2 Some common properties of gases and vapours	26
4.3 The differences between detecting gases and vapours	27
4.3.1 General	27
4.3.2 Detection of gases	27
4.3.3 Detection of vapours	29
4.4 Oxygen deficiency.....	32
4.4.1 General	32
4.4.2 Chemical reaction of oxygen, with solid products	32
4.4.3 Chemical reaction of oxygen, with gaseous products	33
4.4.4 Dilution of the air by displacement by some other gas or vapour	33
4.5 Specific applications of gas detection	34
4.5.1 Gas detection as means of reducing risk of explosion	34
4.5.2 Gas free work permit	36
4.5.3 Monitoring of air inlets	37
4.6 Specific considerations for open path detection	38
5 Measuring principles.....	39
5.1 General.....	39
5.2 Catalytic sensors	41
5.2.1 General	41
5.2.2 Common applications	41
5.2.3 Limitations	41
5.2.4 Interferences	42
5.2.5 Poisoning	42
5.3 Thermal conductivity sensors	43
5.3.1 General	43
5.3.2 Common applications	43
5.3.3 Limitations	44
5.3.4 Interferences	44

5.3.5	Poisoning	44
5.4	Infrared sensors	44
5.4.1	General	44
5.4.2	Common applications	45
5.4.3	Limitations	45
5.4.4	Interferences	46
5.4.5	Poisoning	46
5.5	Semiconductor sensors	46
5.5.1	General	46
5.5.2	Common applications	46
5.5.3	Limitations	47
5.5.4	Interferences	47
5.5.5	Poisoning	47
5.6	Electrochemical sensors	48
5.6.1	General	48
5.6.2	Common applications	48
5.6.3	Limitations	48
5.6.4	Interferences	49
5.6.5	Poisoning	49
5.7	Flame ionization detectors (FID)	49
5.7.1	General	49
5.7.2	Common applications	49
5.7.3	Limitations	50
5.7.4	Interferences	50
5.7.5	Poisoning	50
5.8	Flame temperature analysers (FTA)	50
5.8.1	General	50
5.8.2	Common applications	50
5.8.3	Limitations	50
5.8.4	Interferences	51
5.8.5	Poisoning	51
5.9	Photo ionisation detector (PID)	51
5.9.1	General	51
5.9.2	Common applications	51
5.9.3	Limitations	51
5.9.4	Interferences	52
5.9.5	Poisoning	52
5.10	Paramagnetic oxygen detector	52
5.10.1	General	52
5.10.2	Common applications	52
5.10.3	Limitations	53
5.10.4	Interference	53
5.10.5	Poisoning	53
6	Selection of ~~apparatus~~ equipment	53
6.1	General	53
6.2	Selection criteria	54
6.2.1	General criteria	54
6.2.2	Gases to be detected by the ~~apparatus~~ equipment	55
6.2.3	~~Intended~~ Application of ~~the apparatus~~ fixed equipment	56

6.2.4	Application of transportable and portable equipment.....	60
6.3	Miscellaneous factors affecting selection of ~~apparatus equipment~~	61
6.3.1	Electromagnetic immunity.....	61
6.3.2	Intended Zone(s) of use.....	61
7	Behaviour of gas releases	61
7.1	Nature of a release	61
7.1.1	General	61
7.1.2	Release rate of gas or vapour.....	62
7.1.3	Flammable limits.....	62
7.1.4	Ventilation	63
7.1.5	Relative density of the released gas or vapour.....	63
7.1.6	Temperature and/or pressure.....	63
7.1.7	Other parameters to be considered.....	63
7.1.8	Outdoor sites and open structures	64
7.2	Buildings and enclosures	64
7.2.1	General	64
7.2.2	Unventilated buildings and enclosures.....	64
7.2.3	Ventilated buildings and enclosures.....	64
7.3	Environmental considerations	65
8	Design and installation of fixed gas detection systems.....	66
8.1	~~General~~	66
8.2	Basic considerations for the installation of fixed systems	66
8.2.1	~~General~~	66
8.2.2	~~Point detection equipment and remote sensors~~	67
8.2.3	~~Systems consisting of sampling equipment~~	67
8.2.4	~~Open path (line of sight) equipment~~	67
8.3	Location of detection points	68
8.3.1	~~General~~	68
8.3.2	~~General site considerations~~	68
8.3.3	~~Environmental conditions~~	69
8.4	Access for calibration and maintenance	71
8.5	Additional considerations for sample lines.....	72
8.6	~~Additional considerations for open path equipment~~	73
8.7	Summary of considerations for the location of ~~sensors or sampling~~ measuring points ~~and open paths~~	73
8.8	Installation of ~~sensors~~ measuring point and open path equipment.....	74
8.9	Integrity and safety of fixed systems	74
8.9.1	General	74
8.9.2	Redundancy in fixed systems.....	75
8.9.3	Protection against loss of main power supply.....	75
8.10	Timing of installation during construction operations	75
8.11	Commissioning	75
8.11.1	Inspection.....	75
8.11.2	Initial gas calibration.....	76
8.11.3	Adjustment of alarm set points.....	76
8.12	Operating instructions, plans and records	77
9	Use of portable and transportable flammable gas detection ~~apparatus equipment~~	77
9.1	General.....	77

9.2	Initial and periodic check procedures for portable and transportable instrumentation	79
9.2.1	General	79
9.2.2	Inspection and ~~field functional checks~~ ~~s (response check)~~	79
9.2.3	Routine ~~checks~~ ~~tests~~ and recalibration	80
9.2.4	Maintenance and recalibration	81
9.3	Guidance on the use of portable and transportable ~~apparatus equipment~~	81
9.3.1	Electrical safety in hazardous atmospheres	81
9.3.2	Safety of personnel	81
9.3.3	Spot tests and sampling	82
9.3.4	Sampling above liquids	82
9.3.5	Avoidance of condensation	82
9.3.6	Poisoning of sensors	83
9.3.7	Changes of temperature	83
9.3.8	Accidental damage	83
9.3.9	Minimalist operation, the “Read and run” concept	83
10	Training of operational personnel	84
10.1	General	84
10.2	General training – Basic limitations and safety	84
10.3	Operator training	85
10.4	Maintenance training	85
11	Maintenance, routine procedures and general administrative control	85
11.1	General	85
11.2	Operational checks	87
11.2.1	General	87
11.2.2	Fixed systems	87
11.2.3	Portable and transportable gas detection ~~apparatus equipment~~	88
11.3	Maintenance	89
11.3.1	General	89
11.3.2	Fixed ~~apparatus equipment~~	89
11.3.3	Portable and transportable gas detection ~~apparatus equipment~~	89
11.3.4	Off-site maintenance, general	89
11.3.5	Maintenance procedures	90
11.4	Sensors	90
11.4.1	General	90
11.4.2	Flame arrestor	90
11.5	Flow systems	90
11.5.1	General	90
11.5.2	Inspection	91
11.5.3	Filters, traps and flame arrestors	91
11.5.4	Flow system and sample chamber	91
11.5.5	Flow connections	91
11.5.6	Moving parts	91
11.5.7	Automatic sample-draw systems	91
11.5.8	~~Trouble~~ Loss-of-flow signals	91
11.6	Readout devices	91
11.6.1	General	91
11.6.2	Other readouts	91
11.7	Alarms	92

11.8	~~Workshop calibration test and equipment~~ Calibration	92
11.8.1	Calibration kits and test equipment	92
11.8.2	~~Conduct of workshop calibration testing~~ Calibration procedure	93
Annex A (normative) Measuring principles		95
A.1	General	95
A.2	Catalytic sensors	97
A.2.1	General	97
A.2.2	Common applications	98
A.2.3	Limitations	98
A.2.4	Interferences	99
A.2.5	Poisoning	99
A.3	Thermal conductivity sensors	100
A.3.1	General	100
A.3.2	Common applications	100
A.3.3	Limitations	101
A.3.4	Interferences	101
A.3.5	Poisoning	101
A.4	Infrared sensors	102
A.4.1	General	102
A.4.2	Common applications	104
A.4.3	Limitations	105
A.4.4	Interferences	105
A.4.5	Poisoning	105
A.5	Semi-conductor sensors	105
A.5.1	General	105
A.5.2	Common applications	106
A.5.3	Limitations	106
A.5.4	Interferences	107
A.5.5	Poisoning	107
A.6	Electrochemical sensors	107
A.6.1	General	107
A.6.2	Common applications	108
A.6.3	Limitations	108
A.6.4	Interferences	109
A.6.5	Poisoning	109
A.7	Flame ionization detectors (FID)	109
A.7.1	General	109
A.7.2	Common applications	110
A.7.3	Limitations	111
A.7.4	Interferences	111
A.7.5	Poisoning	111
A.8	Flame temperature analysers (FTA)	111
A.8.1	General	111
A.8.2	Common applications	112
A.8.3	Limitations	112
A.8.4	Interferences	112
A.8.5	Poisoning	112
A.9	Photo ionisation detector (PID)	112
A.9.1	General	112

A.9.2	Common applications	113
A.9.3	Limitations	113
A.9.4	Interferences	114
A.9.5	Poisoning	114
A.10	Paramagnetic oxygen detector	114
A.10.1	General	114
A.10.2	Common applications	115
A.10.3	Limitations	115
A.10.4	Interference	115
A.10.5	Poisoning	115
Annex B (informative)	Environmental parameters	116
Annex C (informative)	Typical environmental and application check-list for flammable gas detectors (for both Group I and Group II equipment)	117
Annex D (informative)	Typical instrument maintenance record for flammable gas detectors	119
Annex E (informative)	Atmospheric visibility (applicable to open path equipment)	121
Bibliography		122
Figure 1	– Integral concentration over the path length.....	38
Figure 2	– Average concentration over the path length	39
Table 1	– Typical Tasks and Most Relevant Causes	12
Table 2	– Overview of gas detection ~~apparatus~~ equipment with different measuring principles	40
Table A.1	– Overview of gas detection ~~apparatus~~ equipment with different measuring principles	96
Table B.1	– Environmental parameters	116

INTERNATIONAL ELECTROTECHNICAL COMMISSION

EXPLOSIVE ATMOSPHERES –

**Part 29-2: Gas detectors – Selection, installation, use
and maintenance of detectors for flammable gases and oxygen**

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as “IEC Publication(s)”). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

This redline version of the official IEC Standard allows the user to identify the changes made to the previous edition. A vertical bar appears in the margin wherever a change has been made. Additions are in green text, deletions are in strikethrough red text.

International Standard IEC 60079-29-2 has been prepared by IEC technical committee 31: Equipment for explosive atmospheres.

This second edition cancels and replaces the first edition published in 2007. This edition constitutes a technical revision.

This edition includes the following significant changes with respect to the previous edition:

Changes	Clause	Type		
		Minor and editorial changes	Extension	Major technical changes
Addition of group 1 to scope	1		x	
Addition of Open Path Gas Detection	3, 4.6, 5.4, 6.2.3.5, 8.2, 8.6, 8.7, 8.8, 11, A4		x	
Changed “combustible” to “flammable”	Throughout	x		
Addition of specific applications	4.5		x	
Improvements to sampling systems	6.2.3.4, 8.2.3, 8.5, 11.2.2	x		

NOTE The technical changes referred to include the significance of technical changes in the revised IEC Standard, but they do not form an exhaustive list of all modifications from the previous version. More guidance may be found by referring to the Redline Version of the standard.

Explanations:

- 1) **Minor and editorial changes** clarification
 decrease of technical requirements
 minor technical change
 editorial corrections

These are changes which modify requirements in an editorial or a minor technical way. They include changes of the wording to clarify technical requirements without any technical change, or a reduction in level of existing requirement.

- 2) **Extension** addition of technical options

These are changes which add new or modify existing technical requirements, in a way that new options are given, but without increasing requirements for equipment that was fully compliant with the previous standard. Therefore, these will not have to be considered for products in conformity with the preceding edition.

NOTE These changes represent current technological knowledge. However, these changes should not normally have an influence on equipment already placed on the market.

- 3) **Major technical changes** addition of technical requirements
 increase of technical requirements

These are changes to technical requirements (addition, increase of the level or removal) made in a way that a product in conformity with the preceding edition will not always be able to fulfil the requirements given in the later edition. These changes have to be considered for products in conformity with the preceding edition.

NOTE These changes represent current technological knowledge. However, these changes should not normally have an influence on equipment already placed on the market.

The text of this standard is based on the following documents:

FDIS	Report on voting
31/1169/FDIS	31/1179/RVD

Full information on the voting for the approval of this standard can be found in the report on voting indicated in the above table.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

A list of all parts in the IEC 60079 series, published under the general title *Explosive atmospheres*, can be found on the IEC website.

The committee has decided that the contents of this publication will remain unchanged until the stability date indicated on the IEC website under "<http://webstore.iec.ch>" in the data related to the specific publication. At this date, the publication will be

- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

IMPORTANT – The “colour inside” logo on the cover page of this publication indicates that it contains colours which are considered to be useful for the correct understanding of its contents. Users should therefore print this publication using a colour printer.

INTRODUCTION

Flammable gas detection ~~apparatus equipment~~ may be used whenever there is the possibility of a hazard to life or property caused by the accumulation of a flammable gas-air mixture. Such ~~apparatus equipment~~ can provide a means of reducing the hazard by detecting the presence of a flammable gas and issuing suitable audible or visual warnings. Gas detectors may also be used to initiate precautionary steps (for example plant shutdown, evacuation, and operation of fire extinguishing procedures).

~~Apparatus Equipment~~ may be used to monitor a gas atmosphere below the lower flammable limit in circumstances where accumulation of gas may result in a concentration of the gas/air mixture to potentially explosive levels. Performance requirements for gas detecting ~~apparatus equipment~~ for such purposes are set out in IEC 60079-29-1 and IEC 60079-29-4. ~~Guidance for functional safety of fixed gas detection systems are set out in IEC 60079-29-3.~~

However performance capability alone cannot ensure that the use of such ~~apparatus equipment~~ will properly safeguard life or property where flammable gases may be present. The level of safety obtained depends heavily upon correct selection, installation, calibration and periodic maintenance of the ~~apparatus equipment~~, combined with knowledge of the limitations of the detection technique required. This cannot be achieved without responsible informed management.

An additional hazard to life is the toxicity of some gases and of the vapours of all liquids except water. It is not generally appreciated that all flammable vapours are potentially toxic at concentration levels which are very small fractions of their respective lower flammable limits. ~~Apparatus Equipment~~ covered by IEC 60079-29-1 and IEC 60079-29-4 is not specifically intended for toxic protection, and additional personal protection precautions will normally be needed where personnel could be exposed to toxic vapours.

Portable ~~apparatus equipment~~ covered by IEC 60079-29-1 and IEC 60079-29-2 commonly have additional detectors for specific toxic gases and also for oxygen deficiency. Users are cautioned that even mild oxygen deficiency may be due to toxic concentrations of some other gas or vapour, which may not be detectable or adequately detected by the ~~apparatus equipment~~ in use.

General requirements for the handbook or manual of any particular flammable gas detection ~~apparatus equipment~~ are specified in IEC 60079-29-1 and IEC 60079-29-4. These standards provide some necessary background knowledge on the points mentioned above.

This standard has been specifically written to cover all the functions necessary ~~to go from the need for gas detection all the way through selection to~~ ongoing maintenance for a successful gas detection operation. Different clauses are appropriate for different tasks within this range of operations. Each clause has been written as stand-alone as far as practicable. This means that some information is repeated in different clauses but with a different emphasis.

Table 1 gives a broad suggestion as to the most relevant clauses to the typical tasks to be performed.

Table 1 – Typical Tasks and Most Relevant Causes

Tasks	Definitions	Basic information properties of gas and vapours	Measuring principles	Selection of ~~apparatus~~ equipment	Behaviour of gas releases	Design and installation of fixed gas detection systems	Use of portable and transportable flammable gas detection ~~apparatus~~ equipment	Training of operational personnel	Maintenance, routine procedures General administrative control	Measuring principles (full detail) (normative)	Environmental parameters (informative)
Function (Clause)	3	4	5	6	7	8	9	10	11	Annex A	Annex B
Authorities	+	+++	+++	+	+	-	-	-	+	-	-
General management	+	+++	+++	+	+	-	-	+	+	-	+
Selection	+++	+++	+	+++	+++	+	++	-	+	+++	+++
Design engineering / management	+++	+++	+	+++	+++	+++	-	-	-	+++	+++
Installation engineering / management	+++	+++	+	++	+++	+++	-	-	-	+++	+++
Installation, technical	++	+++	++	++	++	++	-	-	-	+	++
Commissioning	+++	+++	++	+	++	+++	-	++	+	-	-
Operations management	++	+++	++	+	+	++	++	+++	+++	+	+++
Operation training	+++	+++	+	+	+	+++	+++	+++	+++	+++	+++
Servicing / Calibration	+++	+++	-	-	-	++	++	+	+++	++	++
Repair	++	+++	++	-	-	+	+	+	+++	++	-
“+++” Essential Most appropriate “++” Advisable “+” Useful “-” Not applicable NOTE It should be noted that Clause 5 is a simplified version of Annex A.											

This standard makes recommendations on how to establish maintenance and calibration intervals. In certain countries there are mandatory general or industry-specific regulations ~~that shall~~ which must be followed as a minimum requirement.

EXPLOSIVE ATMOSPHERES –

Part 29-2: Gas detectors – Selection, installation, use and maintenance of detectors for flammable gases and oxygen

1 Scope

This part of IEC 60079-29 gives guidance on, and recommended practice for, the selection, installation, safe use and maintenance of electrically operated Group II ~~apparatus equipment~~ intended for use in industrial and commercial safety applications ~~and Group I equipment in underground coal mines~~ for the detection and measurement of flammable gases complying with the requirements of IEC 60079-29-1 ~~or IEC 60079-29-4~~.

This standard is applicable for oxygen measurement for the purpose of inertisation where explosion protection is provided by the exclusion of oxygen instead of measuring the ~~combustible~~ flammable gases or vapours present. ~~A similar application is measuring oxygen when inertising a goaf (mined out) area in an underground coal mine.~~

This standard is a compilation of practical knowledge to assist the user, and applies to ~~apparatus equipment~~, instruments and systems that indicate the presence of a flammable or potentially explosive mixture of gas or vapour with air by using an electrical signal from a gas sensor to produce a meter reading, to activate a visual or audible pre-set alarm or other device, or any combination of these.

Such ~~apparatus equipment~~ may be used as a means of reducing the risk whenever there is the possibility of a risk to life or property specifically due to the accumulation of a ~~combustible~~ flammable gas-air mixture, by providing such warnings. It may also be used to initiate specific safety precautions (e.g. plant shutdown, evacuation, fire extinguishing procedures).

~~This standard is applicable to all new permanent installations and, where reasonably practicable, to existing permanent installations. It is also applicable to temporary installations, whether new or existing.~~

~~This standard is applicable to fixed installations and transportable equipment. Similarly it is applicable to the safe use of portable or transportable apparatus, irrespective of the age or complexity of such apparatus equipment.~~ Since much modern ~~apparatus equipment~~ of this type also includes oxygen deficiency detection and/or specific toxic gas sensors, some additional guidance is given for these topics.

~~NOTE When in classified areas, the apparatus should be so installed and used that it is not capable of itself igniting a combustible gas-air mixture. It should therefore comply with the requirements of IEC 60079-10.~~

For the purposes of this standard, except where specifically stated otherwise, flammable gases ~~shall~~ include flammable vapours.

Mists are not covered by this standard due to measurement techniques currently used.

This standard applies ~~only~~ to Group II ~~apparatus equipment~~ (i.e. ~~apparatus equipment~~ intended for use in industrial and commercial safety applications, involving areas classified in accordance with IEC 60079-10-1) ~~and Group I equipment~~.

For the purposes of this standard, ~~apparatus equipment~~ includes

- a) fixed ~~apparatus equipment~~ including equipment mounted on a vehicle;

- b) transportable ~~apparatus equipment~~; and
- c) portable ~~apparatus equipment~~.

This standard is not intended to cover, but may provide useful information, for the following:

- a) ~~apparatus equipment~~ intended only for the detection of non-flammable toxic gases;
- b) ~~apparatus equipment~~ of laboratory or scientific type intended only for analysis or measurement purposes;
- ~~c) apparatus intended for underground mining applications (group I apparatus);~~
- c) ~~apparatus equipment~~ intended only for process control applications;
- d) ~~apparatus equipment~~ intended for applications in explosives processing and manufacture;
- e) ~~apparatus equipment~~ intended for the detection of ~~a potentially flammable~~ an explosive atmosphere resulting from dust or mist in air.
- ~~g) open path apparatus not used for point measurement.~~

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

~~IEC 60050-426, International Electrotechnical Vocabulary (IEV) — Chapter 426: Electrical apparatus for Explosive atmospheres~~

IEC 60079-0, ~~Electrical apparatus for explosive gas~~ Explosive atmospheres – Part 0: Equipment – General requirements

~~IEC 60079-10, Electrical apparatus for explosive gas atmospheres — Part 10: Classification of hazardous areas~~

IEC 60079-10-1:2008, Explosive atmospheres – Part 10-1: Classification of areas – Explosive gas atmospheres

IEC 60079-10-2, Explosive atmospheres – Part 10-2: Classification of areas – Combustible dust atmospheres

IEC 60079-13, Explosive atmospheres – Part 13: Equipment protection by pressurized room "p"

IEC 60079-17, Explosive atmospheres – Part 17: Electrical installations inspection and maintenance

IEC 60079-19, Explosive atmospheres – Part 19: Equipment repair, overhaul and reclamation

~~IEC 60079-20, Electrical apparatus for explosive gas atmospheres — Part 20: Data for flammable gases and vapours, relating to the use of electrical apparatus~~

IEC 60079-29-1:2007, Explosive atmospheres – Part 29-1: Gas detectors – Performance requirements ~~of detectors for flammable gases~~

IEC 60079-29-4, Explosive atmospheres – Part 29-4: Gas detectors – Performance requirements of open path detectors for flammable gases

IEC 61285, *Industrial-process control – Safety of analyser houses***3 Terms and definitions**

For the purposes of this document, the terms and definitions given in ~~IEC 60050(426) and~~ IEC 60079-0, as well as the following apply. In addition, since this is intended as a stand-alone standard, certain definitions within IEC 60079-29-1 and IEC 60079-29-4 are repeated below for the convenience of the reader.

NOTE Additional definitions applicable to explosive atmospheres can be found in the International Electrotechnical Vocabulary (IEV), IEC 60050-426.

3.1 Gas properties and other physics**3.1.1****ambient air**

normal atmosphere surrounding the ~~apparatus~~ equipment

3.1.2**clean air**

air which is free ~~of flammable gases and interfering or contaminating substances~~ from gases or vapours (flammable, toxic or environmentally harmful gases) to which the equipment is sensitive or which influence the performance of the equipment

3.1.3**concentration**

amount of the gas or vapour of interest in a specified amount of the background gas or air, expressed in suitable units

Note 1 to entry: Typical units include volume fraction (v/v) (see 3.1.19); molar (moles per mole – m/m); percentage of the LFL of a particular substance; parts per million by volume (ppm); parts per billion by volume (ppb).

3.1.4**dose**

total amount of substance absorbed or trapped, proportional to the concentration and the duration of exposure

3.1.5**explosive gas atmosphere**

mixture with air, under normal atmospheric conditions, of flammable substances in the form of gas or vapour, which, after ignition, permits self-sustaining flame propagation

NOTE 1 ~~This definition specifically excludes dusts and fibres in suspension in air. Mists are not covered by this standard.~~

NOTE 2 ~~Although a mixture that has a concentration above the upper flammable limit (see 3.54) is not an explosive atmosphere, in certain cases for area classification purposes, it is advisable to consider it as an explosive gas atmosphere.~~

NOTE 3 ~~Normal atmospheric conditions include variations above and below reference levels of 101,3 kPa and 20 °C provided the variations have a negligible effect on the explosive properties of the flammable materials.~~

3.1.6**explosive range**

range of gas or vapour mixtures with air, with concentrations between the lower and upper explosive (flammable) limits

3.16**field check with gas (response check)**

~~application of test gas to the sensor to check the response signal or the generation of an alarm, without adjustments of zero, sensitivity, or alarm level~~

3.1.7

firedamp

flammable ~~mixture of~~ gases, consisting mainly of methane, naturally occurring in a mine

3.1.8

flammable gas

gas or vapour which, when mixed with air in a certain proportion, will form an explosive atmosphere

Note 1 to entry: For the purposes of this standard, the term "flammable gas" includes flammable vapour

3.1.9

flashpoint

lowest liquid temperature at which, under certain standardized conditions, a liquid gives off vapours in a quantity such as to be capable of forming an ignitable vapour/air mixture

3.1.10

lower flammable limit

LFL

volume fraction of flammable gas or vapour in air below which an explosive gas atmosphere does not form, expressed as a percentage (see IEC 60079-20-1)

Note 1 to entry: This is also known as lower explosive limit (LEL).

~~3.28~~

~~open path infrared sensor~~

~~sensor capable of detecting gas at any location along an open path traversed by an infrared beam~~

~~3.33~~

~~potentially explosive atmosphere~~

~~atmosphere that could become explosive (the danger is a potential one)~~

~~NOTE This would include an atmosphere with gas concentration currently above UFL (upper flammable limit), where dilution with air would render it explosive.~~

3.1.11

optical radiation

ultra-violet, visible or infrared regions of the electromagnetic spectrum

3.1.12

relative density

density of gas or vapour relative to the density of air at the same pressure and at the same temperature

Note 1 to entry: Air is equal to 1,0.

3.1.13

release rate

quantity of flammable gas or vapour emitted per unit time from the source of release which itself could be a liquid surface

~~3.39~~

~~response check~~

~~see "field check with gas"~~

3.1.14

source of release

point or location from which a flammable gas, vapour or liquid may be released into the atmosphere in such a way that an explosive gas atmosphere could be formed

[SOURCE: IEC 60050-426:2008, 426-03-06, modified by removal of Note]

3.1.15

toxic gas

gas that may be harmful to human health and/or the performance of persons due to its physical or physico-chemical properties

3.1.16

upper flammable limit

UFL

volume fraction of flammable gas or vapour in air above which an explosive gas atmosphere does not form, expressed as a percentage (see IEC 60079-20-1)

Note 1 to entry: This is also known as upper explosive limit (UEL).

3.1.17

vapour

gaseous state of a substance that can reach equilibrium with its liquid or solid state in the temperature and pressure range of interest

Note 1 to entry: This is a simplification of the scientific definition, for the purposes of this standard, and merely requires that the substance is below its boiling point or sublimation point at the ambient temperature and pressure.

3.1.18

ventilation

movements of air and replacement with fresh air due to the effects of wind, temperature gradients or artificial means (for example fans or extractors)

3.1.19

volume fraction

v/v

ratio of the volume of a component gas to the volume of the gas mixture under specified conditions of temperature and pressure

Note 1 to entry: This is also known as volume ratio.

3.2 Types of equipment

3.2.1

alarm only equipment

equipment which generates an alarm signal but does not have a meter or output giving a measure of the integral concentration

3.2.2

aspirated ~~apparatus~~ equipment

~~apparatus~~ equipment that samples the gas by drawing it to the gas sensor – for example by means of a hand-operated or electric pump

3.2.3

continuous duty ~~apparatus~~ equipment

gas detecting ~~apparatus~~ equipment that is powered for long periods of time, but may have either continuous or intermittent sensing

3.2.4

diffusion ~~apparatus~~ equipment

~~apparatus~~ equipment in which the transfer of gas from the atmosphere to the gas sensor takes place by random molecular movement, i.e. under conditions in which there is no aspirated flow

3.2.5

explosion protected ~~apparatus~~ equipment

~~apparatus~~ equipment incorporating a type of explosion protection covered by the IEC 60079 series of standards

3.2.6

explosion protection

measures applied in the construction of equipment to prevent ignition of a surrounding flammable atmosphere by the equipment

3.2.7

fixed ~~apparatus~~ equipment

~~apparatus~~ equipment that is intended to have all its parts permanently installed

3.2.8

group I equipment

equipment for mines susceptible to firedamp

3.2.9

group II ~~apparatus~~ equipment

electrical ~~apparatus~~ equipment for use in places with ~~a~~ potentially an explosive gas atmosphere, other than mines susceptible to firedamp

3.2.10

portable ~~apparatus~~ equipment

spot reading or continuous duty ~~apparatus~~ equipment that has been designed to be readily carried from place to place and to be used while it is being carried

Note 1 to entry: A portable ~~apparatus~~ equipment is battery powered and includes, but is not limited to:

- a) a hand-held ~~apparatus~~ equipment, typically less than 1 kg, which requires use of only one hand to operate;
- b) personal monitors, similar in size and mass to the hand-held ~~apparatus~~ equipment, that are continuously operating (but not necessarily continuously sensing) while they are attached to the user; and
- c) larger ~~apparatus~~ equipment that can be operated by the user while it is carried either by hand, by a shoulder strap or by a carrying harness; which may or may not have a hand directed probe

3.2.11

sample (sampling) system

equipment which typically draws more than one sample, conditions them as necessary, and presents them to a sensor in aspirated equipment

Note 1 to entry: This usually refers to fixed equipment where multiple samples from different detection points are presented sequentially to one or more sensors;

3.2.12

spot reading ~~apparatus~~ equipment

~~apparatus~~ equipment intended to be used for short, intermittent or irregular periods of time as required (typically 5 min or less)

3.2.13

transportable ~~apparatus~~ equipment

~~apparatus~~ equipment not intended to be portable, but which can be readily moved from one place to another

3.3 Sensors and detectors

3.3.1

catalytic sensor

sensor, the operation of which depends upon the oxidation (combustion) of gases on an electrically heated catalytic element

3.3.2

electrochemical sensor

sensor, the operation of which depends upon changes of the electrical parameters of electrodes placed in an electrolyte due to redox reactions of the gas on the surface of the electrodes

3.3.3

flame ionisation detector

FID

sensor, the operation of which depends upon the ionization of the gas being detected in a hydrogen flame

3.3.4

flame temperature analyser

FTA

sensor, the operation of which depends upon the change of temperature of a flame by the gas being detected

3.3.5

infrared absorption sensor

sensor, the operation of which depends upon the absorption of infrared radiation by the gas being detected

3.3.6

paramagnetic oxygen detector

sensor, the operation of which depends upon the magnetic properties of ~~the gas being~~
~~detected~~ oxygen

3.3.7

photo ionisation detector

PID

sensor, the operation of which is based on the ionisation of gaseous compounds by ultraviolet (UV) radiation

3.3.8

remote sensor

sensor that is not integral with the main body of the equipment

3.3.9

semiconductor sensor

sensor, the operation of which depends upon changes of the electrical conductance of a semiconductor due to chemisorption of the gas being detected at its surface

3.3.10

sensor

assembly in which the sensing element is housed that may also contain associated circuit components

3.3.11

sensing element

part of a sensor that reacts in the presence of a flammable gas mixture to produce some physical or chemical change that can be used to activate a measuring or alarm function, or both

3.3.12

single point sensor

sensor capable of detecting gas at a single point location

3.3.13**thermal conductivity sensor**

sensor, the operation of which depends upon the change of heat loss by conduction of an electrically heated element located in the gas to be measured, compared with that of a similar element located in a reference gas cell

3.4 Supply of gas to instruments**3.4.1****measuring point****measurement point**

location of a single sensor aspirated by diffusion or by a probe

3.4.2**point detection equipment**

detection equipment located at a measurement point

Note 1 to entry: This normally refers to a complete single point sensor, rather than a sampling point, and is in contrast with open path equipment

3.4.3**sample line**

means by which the gas being sampled is conveyed to the sensor including accessories

EXAMPLE Filter, water trap.

3.4.4**sampling point**

point from which sample is taken in an aspirated equipment

Note 1 to entry: Typically this term is applied to fixed aspirated systems.

Note 2 to entry: Typically the equipment at this point will consist of a filter, but there may be other sample conditioning equipment as well.

3.4.5**sampling probe**

separate sample line which is attached to the ~~apparatus~~ equipment as required, that may or may not be supplied with the ~~apparatus~~ equipment

Note 1 to entry: It is usually short (e.g. in the order of 1 m) and rigid (although it may be telescopic), but it may be connected by a flexible tube to the ~~apparatus~~ equipment

3.5 Signals and alarms**3.5.1****alarm setpoint**

fixed or adjustable setting of the ~~apparatus~~ equipment that is intended to pre-set the level of concentration at which the ~~apparatus~~ equipment will automatically initiate an indication, alarm or other output function

3.5.2**alarm signal**

audible, visual, electronic or other signal generated by the equipment when an integral concentration of gas in excess of a preset value is detected

3.5.3**continuous or quasi-continuous sensing**

mode of operation in which power is applied continuously to the sensing element and readings are taken continuously or at regular and frequent intervals

3.5.4

fault signal

audible, visual, or other type of output which provides, directly or indirectly, a warning or indication that the equipment is defective or out of adjustment

3.5.5

indicating devices

means for displaying values or states in analogue or digital form

3.5.6

inhibition signal

audible, visual, or other type of output which provides, directly or indirectly, a warning or indication that normal operation has been suspended

3.5.7

intermittent sensing

mode of operation in which the power or flow to the sensor is applied intermittently according to a predetermined cycle and readings taken at the predetermined cycle

3.5.8

latching alarm

alarm which, once activated, requires a deliberate action to deactivate it

3.5.9

safety function

function (inclusive from gas sampling to signal output of the gas detection equipment) to enable the overall system to achieve a safe state.

3.6 Times, checks and equipment behaviour

3.6.1

drift

variation ~~in the apparatus indication with time at any fixed gas volume fraction~~ with time of the indication produced by the equipment under normal conditions when monitoring a fixed gas volume fraction, or, in the case of open path, a fixed concentration distribution, (including clean air) under constant ambient conditions

3.6.2

functional check

application of test gas or other means of obtaining a response from the sensor to check its function

Note 1 to entry: This may include the generation of an alarm. This check is performed without adjustments of sensitivity.

Note 1 to entry: This is also known as a "response check" or "bump test".

3.6.3

initial calibration

first calibration for a specific substance, measuring range and application carried out by the manufacturer before delivery, or on site, before starting the operation

3.6.4

poisons

<for sensors>

substances which lead to temporary or permanent loss of sensitivity of the sensors

3.6.5

recalibration

calibrations carried out periodically to check and adjust the zero signal and the sensitivity of the sensor with a known calibration gas mixture without any changing of the parameters, type of gas, measuring range, specific application, which have been established by the initial calibration

3.6.6

recovery time

time interval between the time when an instantaneous decrease in gas concentration is produced at the sensor input and the time when the response reaches a stated indication

3.6.7

selectivity

response of the ~~apparatus~~ equipment to the gas of interest compared with the response to other gases

Note 1 to entry: If there is high selectivity to the target gas, the results will be less ambiguous and the cross-sensitivity to other gases will be low.

3.6.8

sensitivity

ratio of change produced in the ~~apparatus~~ equipment by a known concentration of gas or vapour

Note 1 to entry: Depending on context, this can refer to the minimum change in concentration of gas or vapour that the ~~apparatus~~ equipment will detect.

Note 2 to entry: High sensitivity implies that low concentrations can be measured.

3.6.9

span

~~upscale~~ reading on the normal test gas of the ~~apparatus~~ equipment

3.6.10

time of response ~~time~~

tx

time interval, with the ~~apparatus~~ equipment in a warmed-up condition, between the time when an instantaneous change between clean air and the standard test gas, or vice versa, is produced at the ~~apparatus~~ equipment inlet, and the time when the response reaches a stated percentage (x) of the stabilised signal on the standard test gas

Note 1 to entry: Not applicable to spot reading equipment.

3.6.11

zero gas

gas recommended by the manufacturer which is free of flammable gases, and interfering and contaminating substances, the purpose of which is calibration/adjustment of the ~~apparatus~~ equipment zero

3.7 Terms exclusive to open path equipment

3.7.1

albedo

proportion of incident light scattered back from a surface

3.7.2

beam blocked signal

audible, visual or other type of output which provides, directly or indirectly, a warning or indication that the optical path is obscured or that the signal detected is too weak to enable the equipment to function normally

3.7.3**gas calibration cell**

sealed enclosure with transparent ends which can be filled with test gases

3.7.4**integral concentration**

mathematical integral of the gas concentration along the optical path

Note 1 to entry: It is expressed in units of concentration multiplied by distance, e.g. LFL metre for flammable gases or ppm metre for toxic gases

Note 2 to entry: 100 %LFL x 1 metre = 1 LFL metre;

10 %LFL x 10 metre = 1 LFL metre.

3.7.5**meteorological optical range****MOR**

length of path in the atmosphere required to reduce the luminous flux in a collimated beam from an incandescent lamp, at a colour temperature of 2 700 K to 5 % of its original value

3.7.6**open path**

optical path which traverses the area (or part of the area) in which the atmosphere is being monitored and through which gases in the atmosphere are free to move

3.7.7**optical axis**

median line of the optical path

3.7.8**optical path**

path traversed by optical radiation from an optical transmitter to an optical receiver

Note 1 to entry: The radiation may traverse the path once, twice or many times depending on the form taken by the instrument

3.7.9**receiver**

assembly in which the optical detecting element(s) are housed and which may contain associated optical and electrical components

3.7.10**retroreflector**

individual or multiple arrangement of reflecting corners of cubes arrayed so that light is reflected back parallel to its incident path

3.7.11**gas detection transmitter**

fixed gas detection equipment that provide a self-conditioned electronic signal or output indication to a generally accepted industry standard (such as 4-20 mA or relay), intended to be utilized with separate gas detection control units or signal processing data acquisition, central monitoring and similar systems, which typically process information from various locations and sources including, but not limited to gas detection equipment

3.7.12**transceiver**

assembly in which the optical detecting element(s) and optical transmitting element(s) are housed and which may contain associated optical and electrical components

3.7.13**transmittance**

fraction of luminous flux which remains in a single beam after traversing an optical path of a given length in the atmosphere

3.7.14**transmitter**

assembly in which the optical transmitting element(s) are housed and which may contain associated optical and electrical components

4 Basic information on the properties, behaviour, ~~and detection of~~ gases and vapours, and specific applications of gas detection

4.1 Detecting gases and vapours — ~~General~~

4.1.1 General

For the purposes of Clause 4, a distinction is drawn between gases, which remain gaseous at typical ambient pressures and temperatures, and vapours where liquid can also exist at any relevant pressure or temperature.

Effective operation of flammable gas detection ~~apparatus equipment~~ depends not only on its performance but also on its correct usage.

~~Apparatus Equipment~~ capability, and its suitability for the intended application and the user's knowledge of its limitations, both generic relating to sensor technology, and individual relating to its other design features, cannot alone ensure that its use will properly safeguard personnel, areas, or locations where flammable gases or vapours may be or are present. The level of safety obtained also depends upon the user having a basic knowledge of gas and vapour properties and phenomena.

This knowledge should enable the user to determine whether the gases are heavier or lighter than air, and whether the vapours are heavier than air or of similar density, and therefore where they may accumulate. If the direction and velocity of air movement is known, it can be seen how they may propagate. In addition, there may be physical or chemical reasons imposing limitations on a particular application, such as calibration considerations.

Consideration ~~has to~~ **shall** be given not only to those gases and vapours that are required to be detected, but also to those gases and vapours that are not required to be detected, but may also be present.

The effects of humidity and temperature variations may need to be evaluated, particularly when sampling lines are used, and, more importantly, if vapours other than water are involved.

Small environmental changes, such as a rise or fall in temperature, which may be ignored for most purposes, can significantly modify conditions, particularly if liquids are present and produce increased amounts of vapours, or if vapours condense as fogs or inside the ~~apparatus equipment~~ itself.

Failure to take these properties of gases and vapours into account at any of the stages of selection, installation, commissioning, training, operation and on-going maintenance of even the simplest of ~~apparatus equipment~~ can result in the production of erroneous readings. These in turn can lead on one hand to false alarms or incorrect action, and on the other hand to failure to alarm or failure to take any appropriate action. Such factors can unnecessarily endanger lives and property.

Some gases or vapours can cause corrosion or other deterioration to certain types of sensors. Some types of sensors have specific lifetimes. The sensitivity can change over time. This applies to certain types of sensors for toxic gases and oxygen deficiency as well as for flammable gases and vapours. This is the major reason for requiring frequent ~~response checking functional checks of some of the more common types of flammable gas detectors~~. It is usually done using a test gas or calibration gas applied in a specified way. The correct test/calibration equipment for one type of gas detection ~~apparatus equipment~~ may not be appropriate to another type, and some training will usually be needed.

Although a mixture that has a concentration above the upper flammable limit is not explosive, it should be realised that on dilution with air it will become explosive, and so it is advisable to consider it as explosive. It should also be noted that it will normally be toxic at much lower concentrations.

4.1.2 Safety when monitoring for flammable gases where personnel could be present

~~When entering the potentially hazardous area frequently observe the readings on the apparatus. Personnel could be entering an already dangerous situation and may need expedient warning.~~

Personnel should frequently observe the reading on any gas detection apparatus when entering a potentially hazardous area. The area may already contain asphyxiates or flammable gas and the personnel may need expedient warning of this danger.

The ~~apparatus equipment~~ will only give a reading for the location where the reading is being taken, or the location of the end of the sampling line if a sampling line is being used. A hazardous atmosphere may be building up a few metres from the sampling point. Therefore, many gas tests ~~must shall~~ be done all around the intended area of work to ensure that no pockets of hazardous gas or vapour are present in the work area.

If vapours are likely to be present, some of the tests should be done one or two centimetres from the floor. This might detect a small problem (e.g. a minor liquid leak) at an early stage. All nearby low spots should be tested.

The readings are only valid for the time they are taken. Circumstances change. Frequent readings are recommended, particularly if vapours (see 4.3.3) could be involved and the temperature is rising.

Where a wide range of gases and vapours could be encountered in the work area there will be a range of potential sensitivities. A low 'alarm point' or 'action point' will therefore be required.

If there is a chance of sensor 'poisons' (such as silicones, leaded petrol, acids, etc.) being present, the sensitivity of an ~~apparatus equipment~~ using catalytic ~~combustion~~ or semiconductor sensors should be checked at frequent intervals.

While the atmosphere is being monitored for ~~flammable properties concentrations~~ of flammable gases and vapours, consideration should also be given to the fact that many of these, including all vapours except water, are also toxic to personnel. Additional detectors for the specific gases and vapours and additional precautions may be needed.

If a flammable gas or vapour detection ~~apparatus equipment~~ is also equipped with high sensitivity sensors for specific toxic gases it should be realized that they may only detect these specific gases. They will not usually detect other toxic materials.

Closely allied to flammable gas monitoring is monitoring for oxygen deficiency and this is detailed in 4.4.1. Frequently this feature is added to the ~~apparatus equipment~~. There are several possible reasons for an oxygen deficiency. Some of them are due to situations where

a toxic substance is part of the cause of the deficiency, and these are of far greater concern. Again, additional detectors and precautions may be needed.

Therefore, when about to work in a hazardous area, it is advisable to specifically check on the potential toxicity of the atmosphere with the plant safety officer, industrial hygienist, or equivalent **and a gas detector that covers the possible range of flammable, and toxic materials in the area should be chosen.**

NOTE Different countries have different systems, and ~~may~~ **can** use different values, for describing maximum safe levels of potentially toxic substances. For typical details, consult the USA's ACGIH book of TLV's (Threshold Limiting Values) and BEIs (Biological Exposure Indices), or the European Commission for the Investigation of Health Hazards of Chemical Compounds in the Work Area who publish a list of recommended TLV's. Both organisations update these publications annually. Other countries usually employ one or the other of these sets of data as a basis for their national documents, which **can** also ~~may~~ be referred to.

4.2 Some common properties of gases and vapours

All gases and vapours will fully mix with all others by diffusion over time or if stirred. They will not separate out. However, some gases and vapours may react chemically with each other on mixing.

If a gas or vapour concentration is increasing in an area it is because more of that substance is being released. It is not due to settling out.

Once gases and vapours have been mixed, they will stay mixed, unless a component is removed chemically, or is absorbed (for instance on a charcoal filter). Additionally, in the case of vapours, removal can be by condensation due to increased pressure and/or falling temperature.

The density of pure gases and the effective density of vapours is proportional to their molecular mass. There is no significant change of volume on mixing gases and vapours. Therefore the density of mixtures of gases and vapours may be simply calculated from the volume fractions and molecular masses of their components. If relative density data is available, the relative density can be similarly calculated from the volume fractions and relative densities of the components.

Air has an equivalent molecular mass of approximately 29, corresponding to a relative density of 1. For instance, gases with lower molecular masses than 29 will have a relative density less than 1 and will be lighter than air.

As an example, methane with a molecular mass of 16 will be lighter than air, carbon dioxide with a molecular mass of 44 will be heavier than air. A mixture of the two, for instance a land fill gas or a mine seam gas, with approximately 53 % methane and 47 % carbon dioxide will have a similar density to air.

Mixtures of ~~fresh clean~~ air with pure or mixed gases that are lighter than air, will still be lighter than air, but less so, **proportionately to their volume fractions**. They will tend to rise until they become so diluted with ~~fresh clean~~ air that the effect becomes negligible.

Mixtures of ~~fresh clean~~ air with gases or vapours that are heavier than air, will still be heavier than air, but less so. They will tend to flow into low spots; pits, trenches etc, until they become so diluted with ~~fresh clean~~ air that the effect becomes negligible.

If a source of release and its surrounding air is substantially hotter than the ambient air the released mixture can rise initially, even if the relative density **at the ambient temperature** is greater than 1. As a rule of thumb, a temperature rise of 30 K will overcome what by calculation would be 10 % greater relative density than air. The converse applies where the release is colder than the ambient temperature.

Because of temperature differences at release and normal turbulence, gases and mixtures with relative density between 0,8 and 1,2 generally can be considered as having a similar relative density to air, and therefore are capable of propagating in all directions.

All flammable gases and vapours will have an LFL and a UFL. The LFL and UFL are experimentally determined, and this data for many substances can be found in IEC 60079-20-1. These values cannot be predicted with any accuracy.

NOTE Because this is experimental, different countries specify different values for LFL and UFL values, which have a legal standing. As two examples:

- NFPA 30 is a publication used within the USA.
- GESTIS is a publicly available database used within Germany.

All vapours, except water vapour, are toxic to varying extents. All flammable vapours are toxic at levels well below 25 % of LFL, most are toxic below 1 % of LFL. At best, gases (except air or oxygen) are asphyxiants (i.e. their effect on personnel is only due to them diluting the oxygen content of the air). Other gases vary from mild to extreme toxicity.

NOTE An asphyxiant is a non-toxic or very mildly toxic and (mostly) inert gas which works by displacing oxygen in the lungs. A toxic gas may cause significant acute health effects even at low concentrations.

When detecting specific gases or vapours, it is necessary to be aware of the potential toxicity of other gases or vapours that might be present, but are not being detected.

4.3 The differences between detecting gases and vapours

4.3.1 General

The major practical differences between the detection of gases and the detection of vapours are outlined below.

4.3.2 Detection of gases

4.3.2.1 General

Substances that remain gaseous under the range of temperatures and pressures relevant to the gas detection application will closely follow the Gas Laws and behave predictably. Basically, simple training ~~will suffice for a normal person may be adequate.~~

Gases may be pure, or any mixture of gases can be made, unless they react chemically. The composition of non-reacting gas mixtures does not change with temperature or pressure.

4.3.2.2 Calibration considerations

Accurate calibration requires calibration gas recommended by the manufacturer for calibration/adjustment purpose which usually contains the target gas in a known concentration with a tolerance of less than 5 % relative. For functional checking, a test gas with reduced accuracy may be used. The manufacturer's recommendations for functional checking of sensors should be followed.

Kits for routine calibration and functional checks of single point sensors, and portable and transportable equipment usually consist of a portable cylinder of a compressed gas, some form of flow control and an adapter to fit the gas detection equipment. In the case of multipoint sampling systems, larger cylinders may be used close to the central equipment, and even permanently connected for automatic calibration.

It is possible to make and store under high pressure, calibration and other test gas mixtures fully representative of the intended gas detection application. Many can be made with a dry or synthetic air ~~background as balance gas. However the more reactive gases tend to have longer storage life if the background is specially dried nitrogen, and this is normally the case.~~

~~unless it is incompatible with the sensor.~~ This is essential for catalytic sensors and others that require air as balance gas in order to operate correctly. However there are safety limits for in compressing gas mixtures that have a volume fraction of more than 50 % LFL.

The more-reactive gases tend to have longer storage life if the balance gas is specially dried nitrogen, and this is normally chosen unless it is incompatible with the sensor.

In order to calibrate open path equipment, a cell with optical windows at both ends containing a calibration gas has to be interposed in the optical path. In order to have practical dimensions for these cells, concentrations of the flammable gas are needed at volume fractions well in excess of the LFL concentrations if they use air as balance gas (see also 4.5). Fortunately the infrared detection principle permits nitrogen to be used as the balance gas, and so the calibration gas may be compressed safely.

Where more than one flammable gas (or vapour) may need to be detected, it is ~~most~~ common to use a single calibration or test gas, and relative response data. For further details see 4.3.3.2.

For calibration gas cylinders the minimum storage temperature specified by the calibration gas manufacturer has to be followed to avoid condensation.

4.3.2.3 Propagation and sampling considerations

Gases can have a density that is lighter than air, such as hydrogen and methane. They can have approximately the same density as air, such as carbon monoxide, hydrogen sulfide, hydrogen cyanide, ethane, ethylene and acetylene; or they can have a density heavier than air such as chlorine, carbon dioxide, sulfur dioxide, LPG, propane, propylene and butane.

When sampling, at least some tests or readings should be taken in locations with the density of the gas in mind. This may also help to detect the source of release.

4.3.2.4 Toxicity considerations

Some flammable gases (specifically ammonia, hydrogen sulfide, hydrogen cyanide, carbon monoxide, methylamine and formaldehyde) are highly toxic at levels which are so low as to be undetectable by conventional flammable gas ~~apparatus equipment~~, although they are listed in IEC 60079-20-1 and can be detected by such ~~apparatus equipment~~ at the much higher levels relevant to detection in LFL ranges. If these gases are likely to be present they will require separate and specific toxic gas sensors, and possibly other precautions, if personnel can be in the area.

Also it is necessary to be aware that some non-flammable gases are highly toxic, such as chlorine, sulfur dioxide, nitric oxide and nitrogen dioxide. If these gases are likely to be present they will require separate toxic gas sensors, and possibly other precautions.

Other flammable gases such as propane, ~~cyclopropane~~, butane and LPG are mildly toxic or narcotic at levels well below their LFL. Similarly non-flammable gases such as carbon dioxide and nitrous oxide are potentially toxic at levels that may not result in a significant oxygen deficiency (see 4.4.4).

4.3.2.5 Water vapour

Although this subclause relates only to detecting gases, it is not normally possible to ignore water vapour. This can produce problems in cold ~~apparatus equipment~~ that have been suddenly exposed to a hotter and humid atmosphere. Examples of this situation are in leaving a cold store and entering a normal atmosphere, or in leaving an air-conditioned situation and entering into a humid tropical or sub-tropical atmosphere. Water can condense in or on a sensor, causing a temporary loss of sensitivity or some other problem, until the ~~apparatus equipment~~ warms up and the water re-evaporates. This is particularly the case with

electrochemical sensors: A very rapid drop in an oxygen reading can occur from a normal 20,8 % or 20,9 % reading to 16 % or lower, due only to a coating of water condensing onto the cold sensor membrane. The sensitivity may then only recover slowly over some minutes as the sensor warms up to ambient, and the film evaporates.

Water vapour may also cause significant deviations of the reading of several types of sensors (see Clause 5 and Annex A).

4.3.3 Detection of vapours

4.3.3.1 General

Vapours are more difficult to understand than gases. Substances, where the liquid or solid can coexist with their gaseous state at normal or slightly abnormal temperatures and pressures are said to have vapours. Vapours behave differently than gases, and can present more problems. Where vapours are likely to be found, additional training in their properties is required.

Where a liquid is present, the rate of evaporation and the maximum volume fraction of the vapour (saturated vapour) will increase with temperature and falling pressure. ~~Similarly the maximum volume fraction of the vapour that can be achieved in a closed system (saturated vapour) will increase with temperature. This is dependent on the temperature and pressure and is~~ The evaporation rate is dependent on the size of the surface of the liquid but independent of the quantity of liquid, provided there is some liquid remaining. The maximum volume fraction of the vapour is also independent of the background gas provided it is at the same temperature and pressure, and is not soluble in the liquid.

The volume fraction that can be reached by the vapour at any temperature is inversely proportional to the absolute pressure. So an increase in pressure can cause condensation.

As a rule of thumb, at constant pressure, the maximum (saturated) volume fraction of any vapour will increase by a factor between 1,5 and 2,0 for each 10 K rise in liquid temperature, and will fall by a factor of 1,5 to 2,0 for every 10 K reduction.

The effect of doubling the absolute pressure has an equivalent effect to a decrease in temperature of 10 K to 17 K at constant pressure. Halving the pressure has an effect equivalent to a similar rise in temperature.

The temperature at which the saturated volume fraction can reach 100 % at the prevailing pressure is the boiling point.

It is only possible to have 100 % volume fraction of a vapour at or above the boiling point at that atmospheric pressure. Below the boiling point of the liquid, the maximum possible concentration of vapour in air or other gases must be less than 100 % volume fraction.

The actual amount of vapour will be less than the amounts predicted above if ~~fresh clean~~ atmosphere is being continually passed over the liquid surface, or if there has not been enough time for equilibration to be established. However this maximum amount can be achieved in an enclosed space, particularly if it has been closed for some time and the air space is slowly stirred by convection or mechanical means.

Flammable liquids have flashpoints, which are determined in a different way from LFL, but are essentially the temperatures at which their vapours can reach their LFL volume fractions in the air above their liquid surfaces, again provided that the vapour is not continuously removed by air currents.

All of these points impose limits on mixtures of vapours with gases. For any particular volume fraction of a vapour in a mixture with gas, a fall in temperature or increase in pressure will, at a certain stage, reach the saturation point, below which liquid will start to condense as a fog

or liquid. When applied to water vapour this is known as the “dew point”. This term is frequently applied to other vapours. Below the dew point the composition of any vapour-gas mixture must therefore change. If this happens within the gas detection system or on the gas sensor, this can lead to falsely low readings on the condensing sample. Also, after such condensation has occurred there will be re-evaporation on returning to cleaner air which will give false high readings.

4.3.3.2 Calibration considerations

Apart from the limitations for gas mixtures in 4.3.2.1, real restrictions on what calibration or test vapours are practical for field use are imposed by the minimum temperature at which they will be used, and the required pressure in a calibration gas or test gas cylinder.

Test kits with a stored pressure in the range 2 MPa to 3 MPa are effectively limited to around 50 % LFL for n-pentane (boiling point 36 °C), about 10 % LFL for n-hexane (boiling point 68 °C), rather less for other substances with similar boiling points, and lower values still for substances with higher boiling points.

Generally, pentane and hexane test gases are directly applicable to the petroleum industry where such vapours can be the main components. However, for other industries, it is seldom possible to make a portable or transportable calibration or test kit for use outside a laboratory that is truly representative of the vapour to be measured.

To get around this problem, responses of the ~~apparatus equipment~~ to different gases and vapours with reference to a particular practical test gas or vapour are determined in a laboratory. Such data is time-consuming and expensive to obtain, and for general purposes is normally only done for a particular model of ~~apparatus equipment~~, not for each unit. In such cases there will be variations between different units.

Routine calibration is then effected in one of two ways:

- a) to give a correct LFL readout on the calibration gas or vapour and use the relative response data directly for the substance(s) of interest (or generate the relative response in software);
- b) to give an artificial LFL readout on the calibration gas or vapour so that the LFL readout will be approximately correct when exposed to the gas or vapour of interest, or to a specified range of gases or vapours.

There can also be variations in relative responses of sensors over time, particularly in the case of sensors which have a ~~definite limited~~ life, or are susceptible to “poisoning” (loss of sensitivity due to chemical action), such as electrochemical and catalytic ~~combustion~~ sensors.

For instance, in the case of catalytic ~~combustion~~ sensors, the response to methane will selectively deteriorate before other gases or vapours. If this happens and the ~~apparatus equipment~~ can be successfully re-calibrated on methane, it will over-read on all other substances, which is in the safe direction.

For this reason, in all catalytic combustion applications where methane could be involved, the use of methane ~~response~~ test gas is recommended for ~~field tests functional checks~~ and during calibration procedures, even if some other gas or vapour is ~~used for the actual calibration the target gas~~. Otherwise propane, ~~butane~~, pentane, or hexane calibration mixtures are usually recommended, for the reason that sensitivity to these will tend to fall before most other substances.

It should also be noted that the sensitivity of catalytic ~~combustion~~ sensors to methane in LFL terms is generally higher than the sensitivity to other substances except hydrogen. Consequently, if using the technique described in a) above, the alarms should be set to a lower set point, and if using the technique described in b) the calibration reading should be set to a correspondingly higher reading than the %LFL of the methane test gas.

Hydrogen ~~should only~~ is to be used as ~~its own~~ calibration gas **only for applications where hydrogen is the only target gas.**

Whenever test or calibration gases other than the gas or vapour of interest are used, it is recommended that additional safety margins, lower alarm settings etc. are employed in order to compensate for the added uncertainty of relative response data due to the factors mentioned above.

4.3.3.3 Propagation and sampling considerations

Only the vapour of water is lighter than air. There are only four vapours, three of which are flammable, with a similar density to air (methanol, hydroxylamine, hydrazine and hydrogen peroxide, the last three being uncommon).

All other vapours are more dense than air. Most are considerably more dense than air. At a point of release, unless heated, they will initially flow downwards or across level surfaces, and until they are well mixed with air they will stay close to the ground, possibly only a few centimetres deep, which is where they will present the greatest flammability problems. A severe instance of this is in the case of pits, trenches and tunnels which will tend to fill from the bottom upwards and can permit extensive propagation over hundreds of metres. This can also cause the most serious toxicity problems for personnel entering pits and tunnels.

When sampling for flammable vapours in relatively undisturbed atmospheres, some tests ~~must~~ **should** be performed at very low levels, ideally within a centimetre of the floor or ground.

Once mixed with an excess of air, all vapours will be found at all levels, possibly at volume fractions well below their LFL but still presenting major toxicity problems

The vapour of a high flashpoint flammable liquid may not be detectable if the ambient temperature is well below the flashpoint. As an example, using the rule of thumb at the beginning of 4.3.3, if the ambient is 60 K below the flashpoint, it can be estimated that the vapour can only reach between 1 % and 8 % of LFL as a maximum, and then only slowly, close to the liquid, and if the vapour is not being blown away.

Conversely, if the temperature rises, and particularly in an enclosed area, the concentration can change dramatically. Again, using the rule of thumb, the vapour concentration in an enclosed space could increase by a factor up to eight for a 30 K rise in temperature, caused, for instance, by the sun on an external tank. A previously undetected amount of vapour while the tank was cold could become very significant when it is heated up. When temperatures are rising, frequent vapour testing is necessary.

Other problems can arise with substances of high molecular mass. The higher the molecular mass is, the lower the rate of diffusion will be. This applies to non-pumped ~~apparatus~~ **equipment** where diffusion screens are used to prevent external ignition, and also within certain sensors. In particular this can adversely affect both the speed of response and the sensitivity in catalytic ~~combustion~~ sensors, ~~particularly the "poison-resistant" varieties.~~

Major problems also arise in vapour testing due to the possible condensation of the sample itself in the detector or its accessories: Gas detectors will only detect the gases or vapours present. They will not detect mists or condensed liquids caused as a result of the ~~apparatus~~ **equipment**, or a sample line, being markedly colder than the atmosphere being sampled.

~~If the apparatus or its sampling line gets contaminated by condensed vapour because it was too cold, or worse still if it gets contaminated by drawing up the flammable liquid, spurious, and possibly dangerously misleading, readings will occur until such contamination is totally removed.~~

If this happens within the gas detection system or on the gas sensor, this can lead to falsely low readings on the condensing sample. Also, after such condensation has occurred there will be re-evaporation on returning to cleaner air which will give false high readings (see 4.3.3.1)

4.3.3.4 Toxicity ~~and other~~ considerations

All vapours except water, including all non-flammable ones, are toxic to some degree. All flammable vapours are toxic at concentrations well below LFL. Most vapours, including many commonly found in industry, are of toxic concern well below 1 % of LFL. Therefore they may be undetectable at concentrations where they are already a toxic problem if only using a ~~combustible~~ flammable gas detector with a normal LFL range. Additional precautions are needed.

4.4 Oxygen deficiency

4.4.1 General

~~Oxygen deficiency detectors are frequently incorporated with flammable gas apparatus, with or without toxic sensors as well. Such oxygen detectors are essential for work in confined spaces.~~

Fixed or portable oxygen detectors are essential for work in locations such as confined spaces and underground coal mines. Portable apparatus typically combine oxygen with flammable gas sensors and frequently also with toxic sensors.

Some varieties of oxygen sensors respond to changes in pressure, and so need checking in ~~fresh~~ clean air, and possibly adjusting, each time they are used and / or if there is a significant change of altitude, ~~such as ascending a tall structure or descending in a mine shaft.~~

The volume fraction of oxygen in dry air is about 20,9 % v/v. A typical oxygen deficiency alarm setting is between ~~19,0~~ 17,0 % to 19,5 % v/v.

Taking as an example a setting of 19,0 % v/v, the alarm should operate on a 1,9 % v/v deficiency or, put another way, a deficiency of 10 % of the original concentration. In certain circumstances (~~presence of toxic gases~~) this may not be adequate for personnel protection.

Similarly, with a setting of 19,5 % v/v, the alarm should operate on a 1,4 % v/v deficiency or, put another way, a deficiency of 7 % of the original concentration. In certain circumstances this also may not be adequate for personnel protection on its own.

~~It is not commonly appreciated that if an operator is relying on apparatus to detect a flammable gas or vapour and a deficiency of oxygen, it is also necessary to know what could be the cause of any Oxygen deficiency found.~~

In many applications the use of a combined apparatus for flammable gases and oxygen deficiency may not provide sufficient information for the operator. Oxygen deficiency may be due to the presence of a toxic gas. In this case, additional detection for toxic gases is required.

There are three basic physical and chemical mechanisms by which oxygen deficiency can occur, described in 4.4.2 to 4.4.4 with reference to the 19,5 % v/v alarm setting example above.

4.4.2 Chemical reaction of oxygen, with solid products

The main examples are the rusting of steel or the corrosion of other metals. Oxygen has simply been subtracted from the air, and a solid oxide is left. This can typically happen in confined spaces constructed of metal.

When the alarm operates at 19,5 % v/v, the atmosphere is equivalent, in physiological terms, to working at an altitude about 650 m higher than the current altitude. Normally this will not cause any health problem to personnel.

4.4.3 Chemical reaction of oxygen, with gaseous products

In the simplest case this could be the result of respiration, aerobic bacterial action (but not anaerobic action), or clean combustion. The 1,4 % reduction in oxygen content needed to set off the alarm would be accompanied by an increase in carbon dioxide level of about 0,8 %, which is fairly safe in the short term, and there would be no short-term or long-term effects on a 'normal person'.

If, however, the oxygen deficiency was the possible result of 'dirty' combustion involving wood, paper, coal, oil, etc, then, even after the smoke had settled, an atmosphere with 19,5 % v/v oxygen remaining could be lethally toxic due to amounts, possibly in excess of 0,2 % v/v (2 000 parts per million), of carbon monoxide produced together with the carbon dioxide.

If the combustion had also involved plastics such as PVC, polyurethane etc, the atmosphere would be very toxic due to additional combustion products such as hydrogen chloride and hydrogen cyanide.

4.4.4 Dilution of the air by displacement by some other gas or vapour

NOTE Detection of a gas by oxygen depletion is only recommended under very controlled conditions and is not otherwise recommended.

The 1,4 % v/v oxygen deficiency needed to cause the alarm would require an addition of 7 % v/v of the other gas or vapour. Thus the problem becomes that of knowing what gas or vapour has caused the deficiency. There are several categories:

a) Inert gases; not toxic

These are further described in the following paragraphs: If the cause of the oxygen deficiency is dilution by one of the inert gases such as nitrogen, argon, helium or neon, (or water vapour) an addition of 7 % v/v or a limited amount more of the inert gas to the atmosphere is perfectly safe. The situation is similar to that in 4.4.2.

NOTE There are areas where the volume fraction of oxygen is controlled at levels between 12 % v/v and 15 % v/v by dilution in this way, to minimise the risk of fire. These areas will be entered in some cases by personnel. If portable oxygen detectors will be used to protect the personnel the alarm levels for the devices have to be specifically adjusted in relation to the oxygen level in those areas. In such cases, for areas with low volume fractions of oxygen personnel have to pass a medical test according to national regulation before being allowed to enter such areas.

b) Flammable gases; not toxic

If the gas causing the oxygen deficiency is hydrogen, methane (natural gas) or ethane, the atmosphere would be safe to breathe for a short period but would be above the LFL, and therefore explosive. But if there was a flammable gas detector as well as the oxygen detector, it should have given an alarm well before this dangerous situation occurred.

c) Flammable gases; toxic

If the gas causing the oxygen deficiency is acetylene, ethylene, ~~cyclopropane~~, propane, LPG or butane, ~~breathing the atmosphere would possibly be survivable by persons working in the area for~~ be lethal within a few seconds at least. But it would be above the LFL. So if there was a ~~combustible~~ flammable sensor as well, this would alarm first.

d) ~~If the gas causing the oxygen deficiency is carbon dioxide, the atmosphere would be marginal. Persons could only stay conscious in such an atmosphere for a short while. A 7 % volume fraction of any other gas or vapour added to the atmosphere, causing that amount of oxygen deficiency, would render the atmosphere potentially and rapidly fatal.~~

Non-flammable; toxic

Oxygen deficiency measurement should never be used for the detection of toxic gases.

WARNING – Oxygen detectors ~~must~~ shall never be used to indicate displacement by CO₂.

Reliance on oxygen detectors to monitor the presence of carbon dioxide has led to fatalities.

~~This may lead to a very dangerous situation. Reliance on oxygen alarms to monitor the production of carbon dioxide has led to fatalities. These were due to confusion between the situation in 4.4.2, where oxygen is subtracted and the alarm operates with around 0,8 % v/v CO₂, and the production of CO₂ by anaerobic processes. The latter situation is covered in this subclause, where CO₂ has been added without subtraction of oxygen, for instance in beer or wine making or by anaerobic slime in manholes. In these cases, the same alarm will not operate until there is 7 % v/v CO₂.~~

~~WARNING – An additional danger in this case is that some oxygen sensors give a small upscale signal with high concentrations of CO₂.~~

~~In the example above, this means that the O₂ reading will be higher than the actual concentration of O₂, and the 19,5 % v/v O₂ alarm would only be given at a significantly higher (and therefore more dangerous) concentration of CO₂ than 7 % v/v.~~

4.5 Specific applications of gas detection

4.5.1 Gas detection as means of reducing risk of explosion

4.5.1.1 General

Flammable gas detection equipment in various combinations of operation may provide means to reduce the probability of an explosion by eliminating sources of ignition (i.e., non-explosion protected equipment that may be located in an area that may be exposed to explosive gas atmosphere) or by activating safety functions to keep flammable gas concentration below 25 % LFL.

In major accidental gas releases, an explosive gas atmosphere is likely to be present beyond the limits of an area classification; and, measures should be taken to eliminate sources of ignition within such areas.

The safety function(s) to be employed by means of gas detection and subsequent actions are:

- a) the disconnection of any non-explosion protected equipment if the set alarm level is exceeded,
- b) increased ventilation rate to prevent increase of gas concentration to above 25 % LFL at the equipment location,
- c) to provide a shutdown signal to the Safety System where detection of flammable gas indicates a loss of containment,
- d) for rooms protected by pressurisation, closure of ventilation dampers to prevent ingress of gas. See also IEC 60079-13 regarding isolation of non-explosion protected equipment inside the room,
- e) for analyser houses, a broad range of provisions as described in IEC 61285, where gas detectors are an important part.

This main alarm level should be at or below 20 % LFL.

In all cases of detection of flammable gas levels at or above 20 % LFL, audible and visual annunciation should be initiated.

Indication of low levels of flammable gas (with or without pre alarm) should be used to:

- 1) initiate troubleshooting and repair activities,

- 2) activate operation of a ventilation system, to increase the rate of existing ventilation to avoid the disconnection of non-explosion protected equipment, and
- 3) shutdown processes due to more severe gas leaks which may cause the exceeding of the main alarm level.

The equipment for the detection of flammable gas should comply with the performance requirements of IEC 60079-29-1 or IEC 60079-29-4 for the gas or vapour likely to be present in the ventilated area.

4.5.1.2 Ventilation Rates

Ventilation and air movement has two basic functions:

- a) To increase the rate of dilution and promote dispersion to limit the extent of a gas hazardous area;
- b) To avoid the persistence of an explosive atmosphere which may influence the type of a Zone

If the ventilation rate is calculated such that gas-air mixtures in concentrations exceeding 25 % of the LFL will not occur this high ventilation rate is the relevant means of protection. Gas detection is not mandatory but is recommended to ensure a high level of safety should the ventilation system fail.

If ventilation rates are considered as low ventilation then a combination of ventilation and gas detection is the means of protection and the recommendations provided should be followed.

All ventilation rates are to be compared with expected flammable gas leakage rates, under various conditions of operation. The relative comparison of ventilation rate to flammable gas leakage rate will determine the manner in which combination flammable gas detection equipment and ventilation should be operated.

Guidance for the assessment of ventilation efficiency and availability can be found in IEC 60079-10-1:2008, Annex B.

4.5.1.3 Gas detection in “high” ventilated areas

In this type of application the primary protection against the accumulation of flammable gas concentrations is by high ventilation. The ventilation rate is calculated such that it is ensured that significant quantities of vapour-air or gas-air mixtures in concentrations exceeding 25 % of the LFL will not occur except in the dilution area.

The ventilation rate should be calculated based on maximum leak rates expected.

The detection of flammable gases is an additional means of protection should the ventilation system fail.

If ventilation fails (a fault condition) disconnection of non-explosion protected ignition-capable equipment should occur.

4.5.1.4 Gas detection in “medium” ventilated areas

If a maximum leak rate cannot be predicted, an adequate ventilation rate may be calculated by assuming leak rates to be expected as realistic. For those leak rates vapour-air or gas-air mixtures in concentrations exceeding 25 % LFL is controlled, resulting in a stable zone boundary, at the ventilation rate determined. However it cannot be excluded that higher leak rates may occur and then the ventilation as the only means of protection will not be sufficient.

Minimum ventilation rates and the ventilation arrangement to be considered must be sufficient to prevent accumulation of flammable gas in corners or behind equipment.

When used in conjunction with medium ventilation rates, equipment for the detection of flammable gases provides an additional level of protection in an area and does form part of the primary safety concept. Gas detection should provide means to cause increase of the ventilation rate at gas concentrations at or below 20 % LFL. If the increased ventilation fails to reduce the vapour-air or gas-air mixtures then the main alarm shall activate the safety function to disconnect all non-explosion protected equipment.

Depending on the local conditions an increase of ventilation should be started at pre-alarm levels between 5 % LFL and 20 % LFL.

If one of the means fails (gas detection or ventilation) the fault has to be indicated. Ignition-capable equipment, can be permitted to operate for a short period if immediate loss of power or automatic shutdown would result in a more hazardous situation, provided repair is initiated and the other means is working correctly.

4.5.1.5 Gas detection in low ventilated areas

Ventilation rates which are so low that they will not prevent the accumulation of flammable gas levels above 25 % LFL are considered as “low” ventilation. In case of low ventilation the degree of dilution may be so low that the classification of the area has a lower Zone number than might otherwise be applied for the grade of release (i.e. a Zone 1 hazardous area from a secondary grade source). Permanent and continuous monitoring of the gas concentration with fixed gas detectors may justify the use of equipment with a lower equipment protection level (EPL) than normally required

For such application both ventilation and gas detection are used as means of protection. Alarm levels and actions (increase of ventilation and disconnection of non-explosion protected equipment) should be the same as in 4.5.1.4.

4.5.1.6 Gas detection in ventilated areas using recirculation

Reduced outside air exchange (below determined adequate ventilation rates) may be used where recirculation of inside air is employed, provided all the following criteria are observed:

- 1) The area is monitored continuously by a gas detection system for flammable gases.
- 2) Flammable gas detection is provided in the return air of the ventilation system.
- 3) When the air inlet flow is reduced, the inside air distribution is maintained by the recirculation.
- 4) The gas detection system will stop the recirculation when exceeding the lowest alarm level (less than 20 % LFL) and increase the ventilation rate for outside air.
- 5) The outside air exchange is provided at a rate that will maintain flammable gas levels below 25 % LFL.
- 6) At the main alarm level at or below 20 % LFL the non-explosion protected equipment shall be disconnected.
- 7) If the ventilation fails the fault has to be indicated but no disconnection of equipment is required, provided repair of the ventilation system is initiated and the gas detection system is working correctly.

4.5.2 Gas free work permit

4.5.2.1 General

In hazardous areas equipment that uses an acceptable method of protection that is required to be temporarily bypassed for maintenance or trouble-shooting, may be operated under a gas free work permit. The work may be performed in a hazardous area with the presence of

protection bypassed under the gas free work permit provided additional equipment for the detection of flammable gas is used and monitored by trained personnel.

NOTE The equipment for the detection of flammable gas can be of portable, transportable or fixed point type detection.

For the maintenance or repair work carried out in a hazardous area, any portable ignition capable devices or equipment (e.g. arc welding equipment, not suitable for the hazardous location) may be operated, according to the work permit instructions and while the equipment for the detection of flammable gas is used and monitored by trained personnel.

The additional equipment for the detection of flammable gas should be suitable for the use in the hazardous area where the work will take place (compliance with IEC 60079-0 and relevant other parts) and should comply with IEC 60079-29-1 for performance for the gas or vapour likely to be present in the working area.

4.5.2.2 Operation

Additional equipment for the detection of flammable gas used to monitor local conditions as a general indication of the presence of flammable gas at the place and time that the permitted work is being performed should be capable of and calibrated for detection of the flammable gas likely to be present in the working area during the time that the permitted work is being performed.

For maintenance and/or repair work of equipment carried out in hazardous areas where the method of protection is bypassed, the following actions should be taken:

- a) All portable/transportable gas detection systems should be checked for functionality with a known concentration of flammable gas just prior to use in conjunction with a gas free permit (bump test).
- b) Initial measurements should be taken to confirm the absence of any flammable gas throughout the work area.
- c) Continuous monitoring should be used to confirm the continued absence of a flammable gas or vapour.
- d) Monitoring equipment should be used and monitored by properly trained personnel.
- e) During any maintenance activity additional and adequate operational procedures should be in place to ensure that the personnel responsible for the emergency response and actions taken when gas presence is detected is able to carry out their duties correctly.

Before the gas free work permit will be given out the points a) and b) should be carried out successfully to certify that a work location is gas free before the method of protection will be bypassed and before the introduction of sources of ignition into that work area will be allowed.

4.5.3 Monitoring of air inlets

Where ventilation air, free of ignitable concentrations of flammable gases or vapours is required (eg. for an air intake for a pressurised room which is located in a hazardous area or internal combustion engine) which is located near areas that may contain explosive gas atmospheres, gas detection to monitor the air inlet should be installed. The following actions should be considered if gas concentrations are detected:

- 1) Shut down the air intake (close dampers and/or de-energize fan supply as appropriate).
- 2) Shut down the process (to halt the release of flammable gas and in preparation for de-energizing the electrical power system).
- 3) De-energize non-explosion protected electrical power system or instruments.

Caution should be exercised when flammable gas sensors are installed inside ventilation air ducts or other turbulent flow applications. This equipment and sensors should be specifically designed, tested, and approved for low level flammable gas detection in turbulent air.

applications to ensure that the actions recommended above will function when flammable gases or vapours are present in the ventilation system.

Where pressurized rooms or houses are located in hazardous areas Zone 1 or 2, they are operated for electrical explosion protection according to IEC 60079-13 and/or IEC 61285. The Clean Air supply used for pressurization should be monitored with flammable gas detectors.

4.6 Specific considerations for open path detection

In Clause 4 so far, concentration units for gases and vapours have been:

- a) percentage volume fraction (% v/v),
- b) lower flammable limit, LFL (also known as lower explosive limit, LEL), which is expressed as a percentage volume fraction specific to a flammable substance, in air,

NOTE For instance the LFL of methane is 4,4 % v/v in air (see IEC 60079-20-1).

- c) percentage of the lower flammable limit, % LFL (% LEL), which is essentially an expression of reciprocal of the safety factor,
- d) parts per million volume fraction (ppm), mainly used in connection with toxic gases and vapours, and flammable gases and vapours in low concentration.

These are the units usually employed in sensor and sampling equipment for oxygen deficiency and for flammable and toxic gases and vapours. At any one time, the sensors use a small, essentially homogeneous, sample which may be in a cell of low volume. Units of concentration are therefore appropriate.

The situation is different in open path equipment which essentially consists of a transmitter and receiver at the ends of an optical path of variable length from 1 metre to 200 metres. The sample is essentially all of the gas in the path between these devices, so it cannot be assumed to be homogeneous in concentration. There is no way of telling if there is a small cloud of high concentration, or a large cloud of low concentration, or more than one cloud. What is measured is the integral concentration over the path length (e.g. in $\text{LFL} \times \text{m}$), as shown in Figure 1, or looked at another way, the average concentration (e.g. in % LFL(avg)) over the path length, as shown in Figure 2.

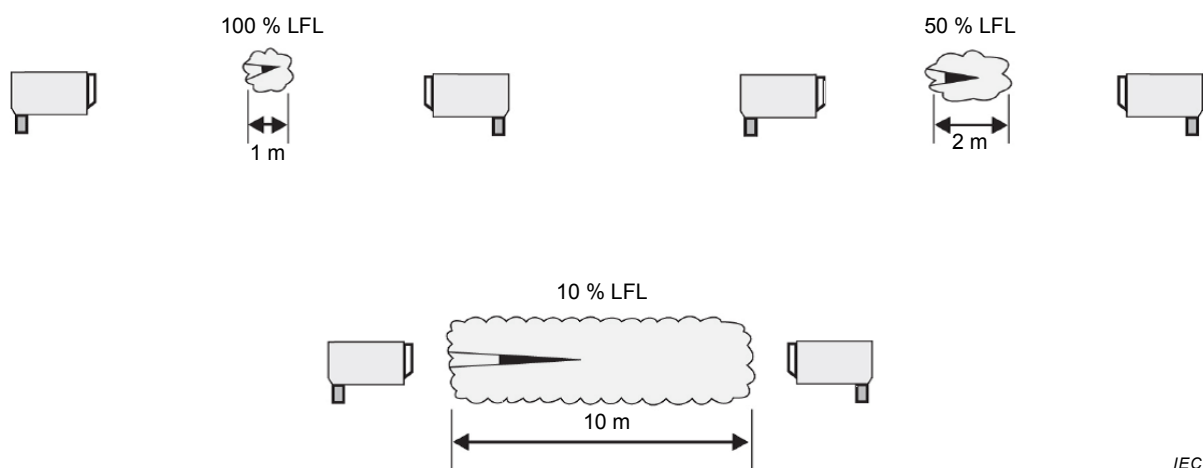


Figure 1 – Integral concentration over the path length

The three Open Path Monitors shown in Figure 1 detail how three gas clouds with different size and concentration would result in the same reading of 1 LFL × m.

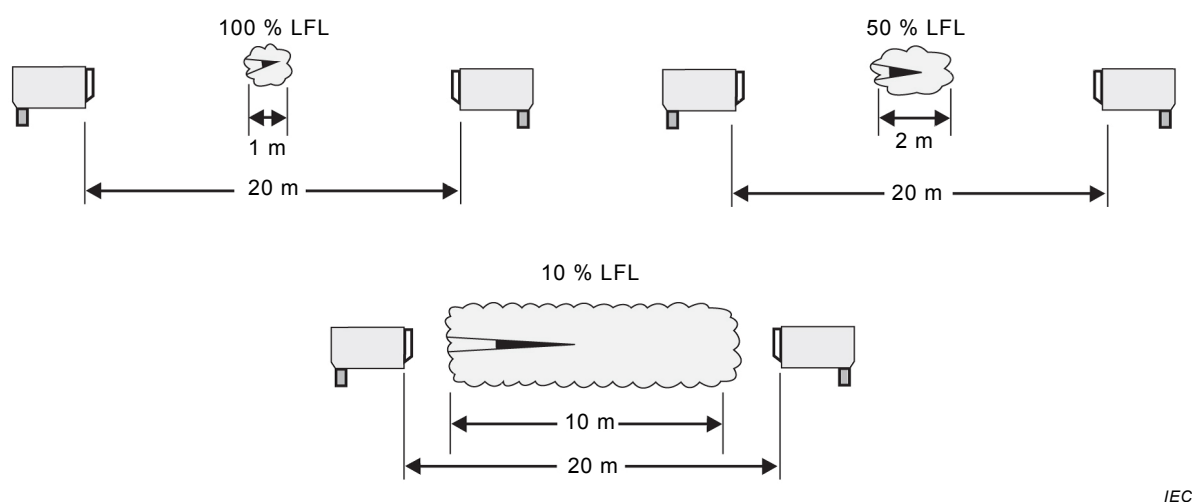


Figure 2 – Average concentration over the path length

The three Open Path Monitors shown in Figure 2 details how three gas clouds with different size and concentration would result in the same reading of 5 % LFL (Path Average Concentration).

5 Measuring principles

5.1 General

~~The measuring principles are handled in full detail in Annex A. This clause is an extract of Annex A to provide practical information for aspects of operation, servicing and repair. Headlines and numbering of subclauses from 5.1 to 5.9.4 are identical with A.1 to A.9.4 of the annex. For more detailed information please use Annex A instead of this clause.~~

Clause 5 is an extract of Annex A to provide an overview of the most important aspects related to the measuring principles. For more detailed information please use Annex A instead of this clause. Titles and numbering of subclauses from 5.2 to 5.10.5 are identical with A.5.2 to A.10.5 of the annex.

It is useful for engineers and managers to know the measuring principles of gas sensors and/or gas sensing elements, when they decide the suitable gas detector for the intended application after talking with manufacturer or seller. However, the performance and function of the gas detector will not be decided only by the gas sensor or the gas sensing element applied to it. Therefore, it should be in mind that the selection of the gas detector should be done considering the total performance and function assisted by the peripheral hardware and software.

The measuring principles of various types of sensors are given below together with their advantages and typical applications and their limitations, interferences by other gases and poisoning (i.e. loss of sensitivity caused by other gases or vapours).

A summary of the most common detection principles is given in Table 2. These are explained in more detail in 5.2 to 5.10 (and in A.5.2 to A.10).

Table 2 – Overview of gas detection ~~apparatus equipment~~ with different measuring principles

	Catalytic sensor	Thermal conductivity sensor	Infrared sensor	Semi-conductor sensor	Electro-chemical sensor	Flame ionisation detector	Flame temperature analyser	Photo ionisation detector	Para-magnetic oxygen detector
Details in subclause	5.2	5.3	5.4	5.5	5.6	5.7	5.8	5.9	5.10
O ₂ required in gas sample	Yes	No	No	(No)	(No)	(No)	Yes	No	Not applicable
Typical measuring ranges ~~Combustible of flammable gases~~	≤ LFL	(0) to 100 % FS	0 to (100) % FS	≤ LFL	≤ LFL	≤ LFL	< LFL	< LFL	Not applicable
Typical measuring ranges for oxygen open path	Not applicable	Not applicable	0– (100) % 0 to 5 LFL × m	Not applicable	0–25 % (0–100 %) Not applicable	Not applicable	Not applicable	Not applicable	0–100 % Not applicable
Typical measuring ranges for oxygen	Not applicable	Not applicable	0 to (100) % FS (with special sensing elements)	Not applicable	0 to 25 % (0 to 100 %) FS	Not applicable	Not applicable	Not applicable	0 to 100 % FS
~~Combustible Flammable~~ gases not measurable	Large molecules	(See 5.3)	H ₂	(See 5.5)	Alkanes	H ₂ ; CO	(see 5.8)	H ₂ ; CO; CH ₄ IP>X ^{5 e}	~~Combustible Flammable~~ gases
Relative response time ^{1 a}	Depends on substance	Medium	(Low)	Depends on substance	Medium	Low	Low	Low	Low to medium
Interference of non-combustible flammable gases ^{2 b}	No	CO ₂ ; Freons	(Yes)	SO ₂ ; NO _x H ₂ O	SO ₂ ; NO _x	ClHCs ^{3 c} ; Halon	(Halon)	Substance IP < X ^{5 e}	NO; NO ₂
Poisoning ^{2 b}	Si; (Hal ^{4 d}); (H ₂ S); Pb	No	No	Si; Hal ^{4 d} ; SO ₂	(No)	(Si)	No	No	No
External gases required	No	No	No	No	No	Yes	Yes	No	(Yes/No)

NOTE 1 ^a Qualitative comparison between principles. The values do not take into account time for aspirated sampling lines.

NOTE 2 ^b Table gives common examples.

NOTE 3 ^c Chlorinated hydrocarbons.

NOTE 4 ^d Organic halogenated or inorganic halogen compounds.

NOTE 5 ^e IP is the ionisation potential of the substance; X is the detector UV-lamp energy.

(No); (Yes) For information on The statements in brackets, refer to the corresponding subclause.

The statements in brackets are conditional and reference should be made to the corresponding subclause.

NOTE The term 'Full Scale' is denoted as "FS".

Alternative detection technologies can be considered. However, the limitations of these alternative technologies should be assessed with respect to their ability or inability to determine the concentration of gas. Therefore, the hazard potential should be clearly understood in a safety system. As a consequence, alternative technologies which do not

comply with gas measurement performance standards (e.g. IEC 60079-29-1 or IEC 60079-29-4) should only be considered as supplementary detection methods. For instance, ultrasonic detectors are available for detection of the presence of leaks particularly from high pressure sources. However, their characteristics are such that the earlier stages of a leak can give a stronger signal than a more developed leak with a higher flow rate. Therefore, such ultrasonic detectors should be regarded as a useful supplement to gas detectors, but in no way should be regarded as their replacement. Another example would be the use of infrared cameras which show location and rough extent rather than the gas measurement concentration.

5.2 Catalytic sensors

5.2.1 General

The principle of operation of catalytic sensors depends upon the oxidation of flammable gas on the surface of an electrically heated catalyst ~~typically operating at a temperature between 450 °C and 550 °C.~~

Catalytic sensors are capable of continuous operation for a few years ~~in the absence of major poisoning,~~ but will progressively drift and lose sensitivity due to ageing and traces of poisons. For this reason regular response checks and recalibration are required, the frequency depending on the severity of the application.

Sensor enclosures in most cases incorporate a permeable metal device to allow gas to reach the sensing element. It also ensures that, if the gas **concentration** is above LFL and ~~is therefore may be~~ ignited by the hot sensing elements, the atmosphere outside the enclosure is not ignited. This protection is also useful against dust or mechanical damage, as well as protection against excessive air velocities.

5.2.2 Common applications

Catalytic sensors are suitable for :

- ~~— the detection in principle of all flammable gases, but with variations in sensitivity;~~
- ~~— the detection of gas/air mixtures up to the lower flammable limit (LFL). They will detect in principle all flammable gases, but with variations in sensitivity.~~

The response time and sensitivity depend on the individual gas to be measured. The larger the molecular mass and molecular size of the gas, the longer will be the response time, and generally, the lower the sensitivity will be.

5.2.3 Limitations

A catalytic sensor ~~depends upon catalytic oxidation for its principle of operation and it functions only when sufficient oxygen (min. 10 %) is present~~ needs sufficient oxygen for its operation. Insufficient oxygen concentration may ~~occur at~~ be caused by high flammable gas concentrations well above the LFL or by inert gases. ~~Therefore, this type of sensor can only be used for the detection of gas/air mixtures up to the lower flammable limit.~~

WARNING – With concentrations above the lower flammable limit, a catalytic sensor may erroneously indicate that the concentration of flammable gas is below the LFL.

Therefore, ~~apparatus equipment~~ fully complying with IEC 60079-29-1 ~~or the former IEC 61779 series,~~ using catalytic sensors ~~must~~ shall have a locking overrange indication to prevent erroneous readouts due to this. However, ~~stand-alone sensors gas detection transmitters~~ (e.g. 4 to 20 mA transmitters) and older ~~apparatus equipment~~ may not provide such protective features.

In case of gas detection transmitters not providing a locking function of the overrange signal the locking shall be provided by the central unit to comply with IEC 60079-29-1.

After exposure to concentrations of gas in excess of the measuring range, ~~or for prolonged periods,~~ the sensor may need a recovery time of several hours or may have irreversible changes to its zero gas reading and sensitivity.

Changes of pressure, temperature and humidity have ~~no significant~~ only limited effect within the specified range. However, the lower the alarm level is set the greater will be the significance of variations in temperature and other environmental factors.

To prevent false alarms, it is recommended that the alarm level should not be set below 5 % LFL for methane, 10 % LFL for propane and butane and 20 % LFL for gasoline vapours, ~~provided suitable precautions are taken against toxicity in the last case.~~

~~For reasons given in the last three paragraphs,~~ These sensors are not suitable for high sensitivity applications (e.g. ranges ~~much~~ less than ~~0~~ 10 % LFL), ~~as amplification would merely amplify these undesirable features.~~

5.2.4 Interferences

~~The measuring principle is generally not selective because all flammable gases (in air) induce a signal. There is a wide variation in sensitivity to different gases which is not directly correlated to the LFL. However, it is possible to use the verified relative sensitivity (as supplied by the manufacturer) for the gas to calibrate the apparatus.~~

~~If the atmosphere to be monitored contains gas or gases that dilute or displace air, for example nitrogen or carbon dioxide, the catalytic sensor may give a low or even zero response. Similar problems may occur in steam-laden atmospheres, quite often owing to saturation of the sintered flame arrester due to condensation. High concentrations of inert gas (for example argon or helium) may also change the thermal balance of the sensor resulting in apparent reading of combustible gas.~~

The response of a catalytic sensor may be lowered by inert gases like nitrogen or carbon dioxide or by condensation of water on the gas inlet e.g. in steam-laden atmospheres.

5.2.5 Poisoning

Catalytic sensors are susceptible to poisoning by ~~traces of several substances~~ ~~many of which are not obviously present but are fairly widely used, necessitating regular response checking and recalibration.~~ This leads to an inhibition which can be permanent or temporary depending on the contaminant.

~~This inhibition may be permanent or temporary according to the nature of the contaminant.~~

~~Permanent inhibition, usually known as "catalyst poisoning",~~ Poisoning may result from exposure to substances as

- silicones (e.g. waterproofing, adhesives, release agents, special oils and greases, certain medical products, ~~commercial cleaning agents~~);
- tetraethyl lead (e.g. leaded petrol, particularly aviation petrol 'Avgas');
- sulfur compounds ~~(e.g. sulphur dioxide, hydrogen sulphide)~~;
- halogenated compounds ~~(e.g. some halogenated hydrocarbons)~~;
- organo-phosphorus compounds (e.g. herbicides, insecticides, and phosphate esters in fireproof hydraulic fluids).

~~In some cases, halogenated hydrocarbons and sulphur compounds may only cause temporary inhibition.~~

So-called "poison resistant" sensors can tolerate higher doses of these contaminants than traditional sensors before they suffer inhibition. In achieving this, their other properties may suffer (e.g. they may have a lower speed of response and reduced sensitivity).

~~Those that are not "poison resistant", in some cases, may be protected against most poisons by the use of activated carbon or other types of filter. However, filters should be used with great care because, while they may offer excellent protection from contaminants, carbon filters in particular will cause a reduced sensitivity to, and may even prevent the detection of, higher hydrocarbons. They also may result in considerably extended response times for substances other than methane or hydrogen, effectively limiting their application to these gases. Filters have a limited lifetime and require replacement. Their performance may also be affected by the level of humidity in the atmosphere.~~

~~The effect of poisoning depends on the poison itself, the gas to be measured and the particular design of the sensor. The manufacturer's guidance should be sought regarding which contaminants may poison the catalyst and how the sensor may be protected.~~

Sensors may be protected against most poisons by the use of filters. However, filters should be used with great care. The advice in Annex A should be followed.

The manufacturer's guidance should be sought regarding which contaminants might poison the sensor and how the sensor can be protected.

5.3 Thermal conductivity sensors

5.3.1 General

The principle of operation of the thermal conductivity sensor depends upon the heat loss by conduction (and sometimes convection or mass transport as well) of an electrically heated resistance element ~~(i.e., filament, bead or thin film resistor) located in a gas sample stream of constant flowrate, or in a diffusion chamber.~~ The sample is not consumed or altered by the sensor, ~~and it does not require oxygen. Therefore, the reading may even be taken with a stopped flow.~~

This type of sensor is suitable for monitoring those gases whose thermal conductivity in the desired detection range differs significantly from that of the reference environment (usually air). ~~However, published tables of thermal conductivity may be misleading as other effects like convection or mass transport also influence the sensitivity of the sensor.~~

5.3.2 Common applications

These sensors do not require oxygen for their operation and are capable of measuring concentrations up to 100 % v/v gas. Typically practical measuring ranges will be well above LFL.

~~The apparatus may be calibrated in any suitable range up to 100 % of a nominated gas in a nominated background gas.~~

These sensors are suitable for detecting an individual gas of high or low conductivity, relative to ~~air, where air is the reference environment~~ a nominated background gas (typically air). High conductivity gases like hydrogen, helium and neon have a good sensitivity in air, and the sensitivity for methane is usually acceptable.

~~The sensitivity is often limited and the minimum practical detection limit may exceed the LFL unless the thermal conductivity of the gas is sufficiently different from that of air.~~

~~A special application is for the purging of LPG tanks with CO₂/N₂ 'inerting' gas. When thermal conductivity is combined with convection it is possible to produce sensors which are largely independent of a range of background gases (e.g. air, nitrogen and certain carbon dioxide / nitrogen 'inerting' gases). At the same time these will respond with at least comparable sensitivities to a range of lower hydrocarbons from methane to pentane, although thermal conductivity data alone would indicate that this is not possible.~~

5.3.3 Limitations

The technique is limited to applications where ~~anticipated~~ variations to the background gas ~~have a negligible effect when~~ are small compared with the response(s) of the gas or gases of interest in the required range.

~~The sensors are not selective for individual gases.~~ The sensors will respond to all gases whether flammable or not.

The thermal conductivities of flammable gases differ widely. Lighter gases (e.g. methane and hydrogen) are more conductive than air whereas heavier gases (e.g. non-methane hydrocarbons) are less conductive. The response to a gas mixture is therefore indeterminate unless the proportions of all the constituent gases in the mixture are known ~~and stable~~. In the worst case, a mixture of high and low conductivity gases could cancel each other out and produce no ~~apparatus~~ response ~~of the sensor~~.

~~Errors may also result if~~

- ~~a) a flow sensitive type of thermal conductivity sensor is used and the gas sample flow is not stable, or if the recommended conditions of gas flow are not maintained as per the manufacturer's instructions;~~
- ~~b) there are variations in ambient temperature without compensatory ambient temperature control on the complete sensor;~~
- ~~c) the apparatus is used in an unintended orientation, particularly if it is a type employing convection as well as conductivity~~

5.3.4 Interferences

~~Interference or errors will be caused if the apparatus is exposed to, or is used to attempt to detect, gases for which it is not calibrated. Specifically additional or unanticipated gases whether flammable or not, of different thermal conductivities to the background can affect the resulting conductivity in either direction, so that the signal may even be reduced to zero.~~

~~Each gas has its individual thermal conductivity and will influence the measurement.~~

A specific interference in many cases is water vapour since it can be highly variable, particularly in hot climates. ~~In the higher sensitivity applications the signal due to likely water vapour variations may be sufficient for the apparatus to require sample conditioning. Sample conditioning may be necessary.~~

5.3.5 Poisoning

There are no known poisoning effects.

5.4 Infrared sensors

5.4.1 General

The principle of operation of ~~spectrophotometric optical~~ infrared sensors depends upon the absorption of energy of a beam of light, ~~in the ultra violet, visible, or infrared parts of the spectrum,~~ by the molecules of the gas being detected. ~~Most existing apparatus operates within the infrared (IR) spectrum.~~

Infrared sensors do not consume the sample, and they do not require oxygen for their operation. ~~They are largely unaffected by flow rate. Sensor life is expected to be long in the absence of corrosion, contamination or mechanical damage.~~

~~The principle of this type of apparatus allows the use of self-diagnostics to verify the response to the gas. Other advantages include~~

- ~~a) high stability capability;~~
- ~~b) no ambiguity at concentrations above the LFL;~~
- ~~c) immunity to poisoning effects;~~
- ~~d) reduced maintenance through self-diagnostics. Automatic calibration, checking capabilities for malfunctions of the infrared source, and compensation for dirt accumulation on the optics, may extend operation periods between service.~~

This type of equipment allows the use of self-diagnostic measures which may extend operation periods between services. However, special consideration should be given to clogging of protective filters in the gas path since this will not normally be detected by self diagnostics.

5.4.2 Common applications

Infrared sensors are calibrated to detect a particular gas or, in some cases, a range of gases. Other gases will not be detected if their infrared absorption band is outside that of the ~~calibration bandwidth sensor.~~ ~~Apparatus~~ Equipment incorporating such sensors should therefore be used only for the detection of ~~gas mixtures~~ ~~gases~~ for which they have been calibrated.

~~Infrared detectors can not respond to hydrogen. However, they may be used for the detection of most other flammable gases, in any specified range of concentration from a few hundred parts per million up to 100 % v/v gas. The longer the optical path is made, the higher will be the sensitivity. Measuring range and performance should be selected according to each application.~~

Typically practical measuring ranges will be from a few hundred parts per million up to 100 % v/v gas. The longer the optical path, the higher the sensitivity will be.

For the IR-measurement of oxygen TDLAS (Tunable Diode Laser Absorption Spectroscopy) devices are used for measuring ranges up to several %v/v or up to 100 v/v.

Typical applications of open path equipment include the lower alkanes, alkenes and alcohols. A typical measuring range is (0 to 5) LFL × m.

5.4.3 Limitations

~~These sensors will not detect hydrogen.~~

Infrared detectors do not respond to hydrogen.

Pressure variations do not affect the zero gas reading, but sensitivity is normally proportional to partial pressure. ~~Since the sensor is sensitive to pressure, care should be taken to prevent alteration to the gas outlet pressure of the apparatus, see instruction manual.~~

Some types of sensor relying on intermittent infrared beams or photoacoustic principles are susceptible to vibration.

~~Some types of infrared sensors, particularly open path designs, are sensitive to misalignment caused by shock and vibration.~~

~~Temperature effects are usually small but may increase or decrease the signal.~~

Open-path designs may be sensitive to misalignment.

5.4.4 Interferences

Other components (~~combustible flammable~~ or non-~~combustible-flammable~~) may induce a signal. ~~Serious errors are likely to occur with some detectors due to interfering gases such as carbon dioxide.~~

Variations of water vapour concentration ~~in the background gas can cause interference with many applications, including general-purpose infrared flammable gas detectors~~ may affect the reading. However, ~~apparatus for this purpose~~ point detection equipment that complies with the requirements of IEC 60079-29-1 will have minimal interference with water.

Solid and liquid contaminants ~~will~~ may also ~~absorb infrared energy, causing~~ cause interference or loss of sensitivity. It is important to prevent contamination of the optical components (e.g. windows and mirrors) ~~by particulate matter or condensation~~. When ~~particulate~~ filters are used to keep optical components clean, ~~they may become blocked under excessively dirty conditions~~ regular maintenance is necessary to prevent blockage.

In the case of open path equipment, the potential effects of water vapour and interfering gases may be much higher. In addition, the equipment has to operate with dust, fog, rain or snow in the optical path, as well as with natural and artificial light. Open path equipment that complies with the requirements of IEC 60079-29-4 will have minimal interference effects on all of these effects.

5.4.5 Poisoning

There are no known poisoning effects.

5.5 Semiconductor sensors

5.5.1 General

The principle of operation of the semi-conductor sensor depends upon changes of electrical conductance that occur by chemisorption ~~of the gas~~ on the surface of the heated sensing element ~~when exposed to gas other than air. Gas concentrations are inferred by measuring the change of resistance.~~

~~The semiconducting material is electrically heated up to a few hundred degrees Celsius. Electrodes are implanted or otherwise mounted on the surface.~~

~~Response times depend on the manufacturing properties of the sensing element, the concentration of the gas to be measured, and the gas transport system to the sensor (mostly by diffusion but aspiration may be used).~~

5.5.2 Common applications

Semiconductor sensors ~~may~~ can be used for the detection of gases ~~over a wide range of concentrations, including very low concentrations,~~ with measuring ranges from the parts per million level up to the LFL and even above. However, they have a non-linear response.

They are suitable for leak detection, even at very low concentrations, and for alarm-only ~~apparatus~~ equipment.

5.5.3 Limitations

Semiconductor sensors for flammable gases are generally non-specific, vulnerable to both humidity changes and interfering gases and may exhibit drift both of zero and span. ~~Some gases, for example NO₂, produce negative signals.~~

~~NOTE Normally, the manufacturer will give guidance on substances that will inhibit operation of the sensor or produce false indications.~~

~~New sensors may need a long "burn in time" (up to weeks) for stabilisation of zero and sensitivity before calibration. This preconditioning should be carried out by the manufacturer. Further preconditioning may be necessary after long periods (> 1 day) without power.~~

Preconditioning of new sensors or after long periods without power may be required, see Annex A.

After exposure to concentrations of gas in excess of the measuring range, the sensor may need a recovery time of several hours or may have irreversible changes to its zero gas reading and sensitivity.

Variations of oxygen concentration, temperature, humidity or air speed may have a strong influence on the sensitivity.

5.5.4 Interferences

The measuring principle is ~~generally~~ not selective. However, improved sensing elements may have some selectivity. Non-combustible flammable gases may induce a negative (e.g. NO₂) or a positive signal.

There ~~is~~ may be a wide variation in sensitivity between sensors of the same type to particular gases and in addition, the relative sensitivities for these gases may vary significantly from one sensor to another. ~~In general, there is a very wide variation in sensitivity to different gases which is not directly correlated to the LFL. Refer to the instruction manual.~~

~~Variations of oxygen concentration, temperature, humidity or air speed may have a strong influence on the sensitivity. Refer to the instruction manual.~~

5.5.5 Poisoning

The sensitivity ~~may~~ can be strongly affected (mostly decreased, but in some cases increased) by poison concentrations higher than those which affect catalytic sensors. Examples of such poisons are:

- basic or acidic compounds;
- silicones;
- tetraethyl lead;
- sulfur compounds;
- cyanides;
- halogenated compounds.

The manufacturer's guidance should be sought regarding which poisons affect the sensitivity of the sensor and how the sensor may be protected.

5.6 Electrochemical sensors

5.6.1 General

The principle of operation of electrochemical sensors depends upon the change of the electrical parameters of electrodes in contact with an electrolyte when a specific gas is present. The change in the electrical parameters occurs due to a chemical reduction / oxidation (redox) reaction of the gas of interest at the surface of an electrode.

The sensors require recalibration at suitable intervals to correct for drifts in zero and sensitivity, and ultimately require replacement. Typical lifetimes under favourable conditions ~~can~~ may exceed 2 years.

5.6.2 Common applications

Electrochemical ~~cells~~ sensors are not available for detecting most hydrocarbons ~~(for example the alkanes, methane, ethane, propane, etc.). However, there are a limited number of applications of this type of sensor for explosion prevention.~~ They are suitable for measuring concentrations of hydrogen or carbon monoxide up to the LFL, and oxygen up to 25 % v/v. There are also sensors available for up to 100 % v/v oxygen.

Additionally, these sensors are commonly used for measuring concentrations of toxic gases down to low parts per million levels. Portable ~~apparatus~~ equipment for the detection of flammable gases, using other types of sensor described in this standard for their (0 to 100) % LFL ranges, frequently have such electrochemical toxic gas sensors and electrochemical oxygen sensors fitted in a multi-gas configuration.

5.6.3 Limitations

~~Temporary, loss of sensitivity occurs in moving a cold sensor of this type into a warmer high humidity situation due to water condensing on the membrane, partially blocking it. This is particularly noticeable on oxygen sensors where a normal reading of just under 21 % can drop for this reason and give an alarm for a few minutes. Contamination by non-volatile liquids or adhesive solids can have a similar but permanent effect.~~

The response of an electrochemical sensor can be lowered by partial blockage e.g. by condensation of water.

Dependent on the sensor, oxygen may be required for the electrochemical reaction. In such cases dissolved oxygen in the electrolyte will last for short periods, but prolonged operation in oxygen-free situations is not possible.

Depending on the type of sensor and the gas to be measured (e.g. oxygen) the sensor ~~may~~ can have a shortened life or a drop in response due to an overload of gas. ~~This can happen particularly with oxygen sensors used in high oxygen concentrations, where a lead electrode is consumed proportionally to the oxygen exposure.~~

~~The lifetime of many types of sensor is also dependent on the dose of other gases because the electrolyte will be consumed. In particular, high concentrations of carbon dioxide can result in loss of sensitivity and shorten the electrolyte life in certain oxygen sensors.~~

Low temperature or humidity ~~may~~ can reduce the sensitivity and increase the response time of the sensor. Prolonged operation in very low humidity can dry out the electrolyte. ~~However, some sensors have a reservoir containing material for maintaining humidity in order to avoid this effect. Electrolyte properties will limit the low (and in some cases the high) temperature operation, see the instruction manual. There is usually a restriction around -15 °C due to potential freezing.~~

~~Response time and recovery time $t(90)$ are comparatively long, typically ≥ 30 s.~~