

IEEE Standard for Automatic Meter Reading Via Telephone—Network to Utility Controller

1. Overview

1.1 Scope

This standard describes the telephone network interface to a utility controller operating under the utility telemetry service architecture. The utility telemetry architecture is a basic transport architecture capable of supporting many different applications. Telemetry calls may be initiated from either the utility/enhanced service provider or the telemetry interface unit on the end user's premises. The two access methods defined for this service are the central office service unit access method and the direct dial access method. The two telemetry interface unit transmission methods defined for this service are the off-hook transmission method and the on-hook transmission method. The interface covered in this standard is described in terms of a basic utility meter-reading/controlling service. However, any number of other applications can be delivered using the telemetry transport service.

1.2 Purpose

The purpose of this standard is to provide a generic interface to a utility controller that is supported by the architecture of the utility telemetry service. The architecture will provide utilities a facility that is readily available, has short setup times, and allows for automatic meter reading using the capabilities of the switched telephone network. The architecture and interface will also support a multitude of different transport applications for other industries.

2. References

This standard shall be used in conjunction with the following publications. If the following standards are superseded by an approved revision, the revision shall apply.

ANSI T1401-1993, American National Standard for Telecommunications—Interface Between Carriers and Customer Installations—Analog Voicegrade Switched Access Lines Using Loop-Start and Ground-Start Signaling.¹

¹ANSI publications are available from the Sales Department, American National Standards Institute, 11 West 42nd Street, 13th Floor, New York, NY 10036, USA (<http://www.ansi.org/>).

Canadian Department of Communications CS-03: 1998, Terminal Equipment, Terminal Systems, Network Protection Devices, Connection Arrangements, and Hearing Aids Compatibility.²

Federal Communications Commission Rules and Regulations, Title 47, Part 68, Connection of Terminal Equipment to the Telephone Network.³

IEEE Std 820-1984 (Reaff 1992), IEEE Standard Telephone Loop Performance Characteristics.⁴

IEEE Std 1390-1995, IEEE Standard for Utility Telemetry Service Architecture for Switched Telephone Network.

IEEE P1390.2/D1, 26 March 1997, Draft Standard for Automatic Meter Reading Via Telephone—Network to Telemetry Interface Unit.⁵

3. Definitions, abbreviations, and acronyms

3.1 Definitions

Terms used in this standard are defined relative to their usage with respect to the architecture and interfaces of a basic utility telemetry service. IEEE Std 100-1996, The IEEE Standard Dictionary of Electrical and Electronics Terms, should be referenced for terms not defined in this clause.

3.1.1 abbreviated ringing: A short, variable burst of power ringing that is required to establish a temporary communications path in certain types of network pair-gain equipment. The switch is instructed, via trunk signals, to output this abbreviated ringing on the end user's line.

3.1.2 alert tone: A non-power ringing tone, or combination of tones, used to request the telemetry interface unit (TIU) or customer premise equipment (CPE) to become active.

3.1.3 alert tone code: A data byte that identifies which alert tone is to be used by the central office service unit (COSU).

3.1.4 automatic call distribution (ACD): A service that evenly distributes calls among incoming end user lines.

3.1.5 automatic number identification (ANI): A network service that delivers the phone number/billing number of the calling party.

3.1.6 call-type information (CTI) digits: Digits sent to the switch from the central office service unit (COSU) via signaling on the utility telemetry trunk, per call, which specify the customer premise equipment (CPE) transmission interface (i.e., on-hook or off-hook operation). These information digits are assigned, on a trunk group basis, through the switch administration procedures.

²This document is available from Global Engineering, 15 Inverness Way East, Englewood, CO 80112-5704, USA, tel. (303) 792-2181 (<http://www.global.ihs.com/>).

³FCC documents are available from the Federal Communications Commission, 445 12th Street S.W., Washington, D. C., 20554. Title 47 is freely available via the web at <http://www.fcc.gov/wtb/rules.html>.

⁴IEEE publications are available from the Institute of Electrical and Electronics Engineers, 445 Hoes Lane, P.O. Box 1331, Piscataway, NJ 08855-1331, USA (<http://www.standards.ieee.org/>).

⁵This IEEE standards project was not approved by the IEEE-SA Standards Board at the time this publication went to press. For information about obtaining a draft, contact the IEEE.

3.1.7 central office service unit (COSU): A telephone company controller resident in a central office that connects to the utility controller and, via the utility telemetry trunk, to the switch. The COSU provides the function of originating and terminating calls to and from telemetry interface units (TIUs). For the COSU access method, the COSU performs a security check with the utility controller and places a call to the end user in response to the information sent to it by the utility controller. The COSU performs a security check and initiates a connection to the utility controller when called by the TIU. The COSU also provides a multiplexing interface between the utility controller and COSU and the COSU and TIU(s). The COSU may also provide traffic measurements.

3.1.8 central office service unit (COSU) access method: An access method that utilizes the switched telephone network, comprised of a COSU, switch, and other network elements. This method provides for automatically invoking/ignoring certain switch-based telemetry communications capabilities and establishes a communications path between a utility/enhanced service provider (ESP) and a telemetry interface unit (TIU).

3.1.9 customer premise equipment (CPE): Equipment located on the customer's premise that is connected to the telephone line [e.g., telemetry interface unit (TIU), telephone, answering machine, modem].

3.1.10 customer premise equipment (CPE) active state: Occurs when the CPE has been alerted and is performing a communication function.

3.1.11 customer premise equipment (CPE) inactive state: Occurs when the CPE has completed its communication function.

3.1.12 cut-through: A transmission path through the switched telephone network to an end user.

3.1.13 digital loop carrier (DLC): Equipment that increases the number of end users served by existing loop side pairs by the use of digital multiplexing. These concentration systems are often called pair gain devices. Both universal and integrated DLCs may be used.

3.1.14 direct dial access method: Utilizes the switched telephone network, comprised of a switch and other network elements that establish a communications path between a utility/enhanced service provider (ESP) and a telemetry interface unit (TIU).

3.1.15 enhanced service provider (ESP): A service provider offering services through the telephone network using the telemetry transport capabilities to deliver their services.

3.1.16 in-band tones: Typically, a signal on the communication path in the range of 400–3300 Hz.

3.1.17 inbound telemetry: Communication initiated by a telemetry interface unit (TIU) toward a utility or enhanced service provider (ESP).

3.1.18 incoming calling line identification (ICLID): Provides calling party data on calls originated from both analog and digital lines.

3.1.19 independent telephone company: A company not associated with a regional Bell operating company (non-Bell operating company).

3.1.20 local access and transport area (LATA): A local telephone exchange area that serves to distinguish local phone service from long-distance phone service. Customers are served by a regional Bell operating company (RBOC) or other telephone company (OTC).

3.1.21 local loop: The communication path between the telephone company's switching office and the end user.

3.1.22 loop current feed open (LCFO): A Bellcore-defined, switch generated, fixed open (no voltage) on the line within the range of 150–350 ms as sent by the switch. Its purpose is to signal certain digital loop carrier (DLC) devices to assign a time slot (transmission path) for a 15 s interval.

3.1.23 modified calling line disconnect: A telephone network feature that, if the end user is off-hook, requires the end user's line to go on-hook before receiving a dial tone from the telephone network.

3.1.24 multiline hunt group (MLHG): A group of lines that have a fixed alternate routing should one or more of the lines in the group be busy.

3.1.25 network interface (demarcation point): The point of connection between the local loop and the end user's (customer provided) wiring.

3.1.26 no-test trunk: A specialized switch facility used by the operator and service personnel for metallic testing of a subscriber's telephone lines (also known as a test trunk facility).

3.1.27 no-test trunk access method: Used to connect to an end user's line, the no-test trunk access method contains a direct metallic path and is primarily used for loop and customer premise equipment (CPE) testing purposes.

3.1.28 on-hook/off-hook: Signaling conditions on a line in the form of dc impedance presented to the local loop by the telemetry interface unit (TIU). Off-hook implies that the TIU is in a low resistance state and is allowing significant current to flow. On-hook implies that the TIU is in a high resistance state and is not allowing significant current to flow. See ANSI T1401-1993 and the local access and transport area (LATA) Switching Systems Generic Requirements (LSSGR), Section 6.2.2, Bell Communications Research (Bellcore) for more detail.

3.1.29 outbound telemetry: Communication initiated by a utility or an enhanced service provider (ESP) toward a telemetry interface unit (TIU).

3.1.30 polarity guard: A device that guarantees proper tip/ring polarity.

3.1.31 post disconnect timing: A timing interval (normally about 12 s in length), initiated when the called party goes on-hook, in which the established connection remains in place as long as the calling party continues to remain off-hook.

3.1.32 regional Bell operating company (RBOC): A regional telephone company that may or may not be made up of individual operating companies.

3.1.33 technical advisory (TA): A telephone company publication intended to disclose information and request comments regarding network services.

3.1.34 telemetry interface unit (TIU): A customer premise equipment (CPE) device that provides a network gateway function and an interface to one or more meters (water, gas, and electric), other telemetry/control devices, or to a local area network. The TIU may be placed in series with or bridged onto the local loop assigned to the end user. Because the TIUs are not network elements, but are regarded as CPE, they are connected to the end user's line (tip/ring) of the local loop at the network interface. In existing systems, these units are also known as meter interface units (MIU).

3.1.35 technical requirements (TR): A telephone company publication intended to disclose information and operation regarding network services.

3.1.36 utility controller (UC): A controller resident on a utility or enhanced service provider (ESP) premise that connects, via the telephone network, to the telemetry interface unit (TIU) (using the direct dial network

access method) or the central office service unit (COSU) (using the COSU network access method or the no-test trunk network access method).

3.1.37 utility telemetry trunk (UTT): A two-way telephone company facility connecting the central office service unit (COSU) to the switch. This facility allows a utility or enhanced service provider (ESP), via the telephone network (COSU), to automatically invoke/ignore certain telephone network capabilities as well as provide a suppressed or abbreviated ringing access to telemetry interface units (TIUs) on an end user's line. The TIU may also originate calls through the telephone network (COSU and switch), which will automatically invoke/ignore certain telephone network capabilities and provide a connection to the utility or ESP.

3.1.38 wink: A momentary off-hook condition in telephone trunk signaling. A wink may have different meanings depending on where it is used in the signaling stream (i.e., start or connect).

3.2 Acronyms and abbreviations

ACD	automatic call distribution
AMR	automatic meter reading
ANI	automatic number identification
COSU	central office service unit
CPE	customer premise equipment
CTI	call type information
DLC	digital loop carrier
ESP	enhanced service provider
LATA	local access and transport area
LFCO	loop current feed open
LSSGR	LATA Switching Systems Generic Requirements
MIU	meter interface units
MLHG	multiline hunt group
NI	network interface
OTC	other telephone company
RBOC	regional Bell operating company
TA	technical advisory
TIU	telemetry interface unit
TR	technical requirements
UC	utility controller
UTS	utility telemetry service
UTT	utility telemetry trunk

4. Utility telemetry service description

4.1 Feature description (Figure 1)

The analog feature allows for the transport of data between a utility or an enhanced service provider (ESP) and an end user's telemetry interface unit (TIU) or other customer premise equipment (CPE) device attached to the telephone line. Communications may be established by the utility/ESP or TIU. Communication connections from the utility/ESP to the telephone network shall utilize the switched network, private networks, packet networks, or telephone company gateways with combinations of networks set up for efficient communications.

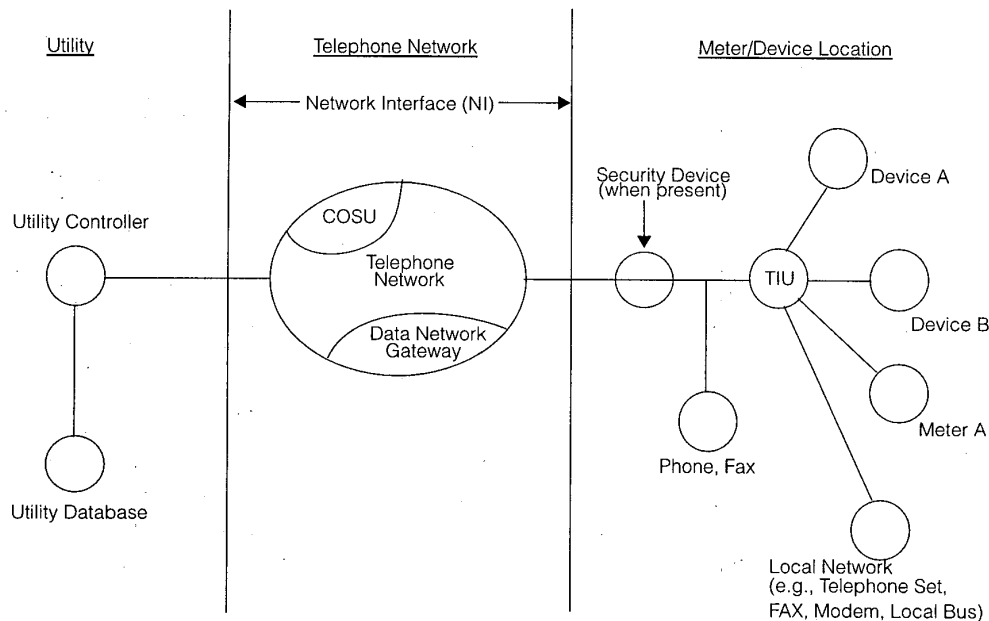


Figure 1—Utility telemetry service architecture for telephone network communications

Automatic meter reading (AMR) is used to describe the utility telemetry service (UTS). AMR is the most popular use for the UTS feature today. There are, however, other applications that will take advantage of a suppressed ringing end user access or a CPE device that initiates calls from the end user's premise. An example of utility-initiated (outbound) applications could include utility-initiated direct control of remote devices (i.e., resource shut-off), ESP-initiated messaging (i.e., voice mail message waiting notification), or ESP-initiated appliance diagnosis. Examples of TIU-initiated (inbound) calling devices are end-user security systems, end-user medical alert systems, utility load control systems, and smart appliances. Smart appliances may initiate calls to service bureaus based on internal maintenance routines or to provide usage-sensitive billing. Calls to the utility/ESP may also be connected to telephone-company-provided multiline hunt groups or automatic call distribution (ACD) services for more efficient communications capability.

The telephone end user whose line is being used for UTS is typically not alerted (i.e., by an audible signal) that a utility telemetry call is in process. Also, calling priority is always given to the end user. When the utility or ESP calls the TIU using the central office service unit (COSU) access method, the end user's line is alerted by a signal that does not operate the end user's CPE ringer. The direct dial access method will cause the end user's ringer to be operated. Additionally, the TIU must go on-hook (off-hook transmission method) or go to the idle state (on-hook transmission method) if the end user goes off-hook (except for security devices, as described in other sections). The end user will only become aware of the utility/ESP call if dialing or data transmission is heard or a delayed dial tone is detected.

Various components and protocols of the UTS are the subject of other IEEE standards (e.g., IEEE Std 1390-1995; IEEE P1390.1/AMR.5/99-001, 3 February 1999; IEEE P1390.2/D1, 26 March 1997).

Multiple TIUs, as well as other end-user CPE, may be present on a single end user's line. Each TIU may access one or more ports, which are connected to the devices requiring communications capability.

To completely describe the progress of the telemetry call and the differences between the identified network access methods, it is important to describe certain internal telephone network operations. Internal telephone network operations are controlled by the local telephone company and are fully defined in local telephone company technical documents.

4.2 Telephone network access methods

The COSU access method and direct dial access methods shall coexist with each other and one TIU may implement both access methods.

4.2.1 COSU access method

When the COSU access method is utilized, the utility controller may use a variety of connections to the telephone network. Examples of these connection methods are switched network connection to the COSU network element, a direct connection, a high-speed digital connection, or a network gateway element. The choice of connection methods is engineered by the telephone company and utility, based on expected traffic and other parameters to provide for efficient communication.

The call shall be handled by the COSU-switch combination, which shall allow for automatic invoking/ignoring of certain switch-based telemetry communications capabilities. For example, this access method will provide a connection to a line that has a valid directory number but the connection has been denied because of vacation service or financial reasons. These communications capabilities are covered by the technical documents issued by regional Bell operating companies (RBOC) or independent telephone companies.

4.2.2 Direct dial access method

When the direct dial access method is utilized the utility controller will only use the switched telephone network to connect to the TIU.

The call shall proceed through the existing switched network and activate those communications capabilities that can be activated by the end user. The call may be affected by network features assigned to the line. For example, the TIU may activate/deactivate selected telephone network (switch) features assigned to the end user's line, as an end user would, with a sequence of dialed digits for each feature. These communications capabilities are covered by the technical documents issued by a RBOC or an independent telephone company.

4.3 Call initiation by utility or ESP

4.3.1 Using the COSU access method

The utility controller will access the telephone network via the chosen telephone network access. A communications path will be established between the utility controller and the telephone network (COSU). A security dialog will take place. If the security dialog is successful, the call will be connected using the COSU network element. The telephone network (COSU) will establish a suppressed ringing connection to the end user's line, allowing communications with the TIU. The TIU shall be alerted by the telephone network [using alert tone(s) and subaddresses]. Data is exchanged in either direction. When the data exchange is completed, the telephone network (COSU) causes the telephone network (switch) to disconnect from the end user's line.

4.3.2 Using the direct dial access method

The utility controller will access the switched telephone network and dial the TIU directly using the standard telephone network capabilities. Several defacto techniques have been implemented to cause the TIU to become active and either answer the call or dial back to the utility/ESP.

4.4 Call initiated by the TIU

The TIU initiates a call by going off-hook and dialing a preprogrammed series of digits. With either the COSU access method or the direct dial access method, the call shall be connected, via the telephone network, to the utility or ESP. Data is exchanged in either direction and the call is disconnected.

4.5 TIU transmission methods

4.5.1 Off-hook transmission method

When the off-hook transmission method is utilized, and the TIU is alerted or wakes up and becomes active, the TIU goes off-hook, causing a bidirectional communications path to be established through loop-side elements and the switch. While the TIU is communicating, the TIU is off-hook. During communications, the switch cannot detect multiple off-hook signals from the end user's line (the TIU is already off-hook). Should the end user go off-hook during a telemetry call, the TIU or telephone network (COSU) must detect the end user's off-hook condition and cause action to disconnect the utility call.

4.5.2 On-hook transmission method

When the on-hook transmission method is utilized, and the TIU is alerted or wakes up and becomes active, the TIU remains on-hook and becomes active. The telephone network assumes a bidirectional communications path to be established through selected loop-side elements and the switch. While the TIU is communicating, the TIU is on-hook. Should the end user go off-hook during a telemetry call, the telephone network (switch) will detect the end user's off-hook signal and cause action to disconnect the utility call. The telephone network (switch) is able to detect this off-hook signal since there are no other TIU (or other CPE devices) in an off-hook state on the end user's line.

4.6 Telephone network technical requirements (TRs)

There are no Bellcore technical advisories or technical requirements on this subject.

The RBOC technical advisories/technical requirements documents are listed in Table 1.

5. Utility controller unit functional requirements

5.1 Controller description

The utility controller is a device that resides on the premises of the utility or ESP. On one end, the utility controller is connected to the telephone network through a variety of standard data connection means. On the other end, the utility controller may be connected to the utility operations computers. The utility controller may or may not be connected to other utility or ESP components.

IEEE Std 1390.3-1999 standardizes the utility controller interface to the telephone network. The utility controller itself may be the subject of separate standards.

Existing TIUs, called meter interface units (MIUs), may continue to be used and may coexist with the UTS. Existing TIUs (MIUs) are not described in this standard. The utility controller may have to support the existing TIUs.

Table 1—RBOC Technical Advisories/Technical Requirements documents

Company	No-test trunk no.	UTS no.	Title
BellSouth	TR 73547	TA 73565	Automatic meter reading services network interface specification
Bell Atlantic	TR 72015	—	BellAtlantic automatic meter reading service interface specification
Ameritech	TR MKT 000035	AMTA-TMO-000098	Ameritech automatic meter reading service interface specifications
NYNEX	NTR-74310	—	Meter reading access arrangement
Southwestern Bell	draft dated 12/90	—	—
US West	77328	—	Automatic meter reading service interface specifications

5.2 Functional requirements of the utility controller

5.2.1 General

The utility controller must conform to all U.S. Federal Communications Commission (FCC) regulations or Canadian Department of Communications regulations that are appropriate for this type of device.

The utility controller must conform to the regulations of the operating companies serving the end user's line.

5.2.2 Physical

The utility controller must connect to the telephone network (COSU) via standard data connections (switched network, packet network, high-speed digital network, network gateway, or private line). These connections are described in IEEE Std 1390-1995; IEEE P1390.1/AMR.5/99-001, 3 February 1999; and IEEE P1390.2/D1, 26 March 1999.

The utility controller connection to the utility operations computers may be the subject of other IEEE standards (e.g., IEEE Std 1390-1995; IEEE P1390.1/AMR.5/99-001, 3 February 1999; and IEEE P1390.2/D1, 26 March 1999).

5.2.3 Link

The TIU is alerted by the telephone network (COSU) based on parameters passed to the telephone network (COSU) by the utility controller.

With the COSU access method, the utility controller will initiate communications by going off-hook, becoming active, and presenting the following:

- Directory number
- TIU identifier
- On-hook and off-hook TIU transmission type
- Identification of the proper alert frequency
- Subaddress (if present)
- Abbreviated ring duration or loop current feed open parameter to the telephone network (COSU)

With the direct dial access method, the utility controller will initiate communications by going off-hook, becoming active, and dialing a directory number.

A dial-back connection or other technique may be implemented for security between the utility controller and the telephone network (COSU). The security dialog is the subject of a future standard.

Both off-hook and on-hook TIU transmission methods are covered in this standard as well as IEEE Std 1390-1995; IEEE P1390.1/AMR.5/99-001, 3 February 1999; and IEEE Std 1390.2/D1, 26 March 1997.

The utility controller/telephone network (COSU) and telephone network (switch)/TIU protocol interworkings are defined in the IEEE P1390.1/AMR.5/99-001, 3 February 1999; telephone company technical requirements; and other specifications.

The telephone network (switch) will enforce the maximum TIU/COSU connect time as defined by the telephone company service provider.

The utility controller must support either a network connection to the telephone network (COSU) or a network connection to a network gateway.

With the COSU access method, if alerted with power ringing, the utility controller shall go off-hook and become active.

With the direct dial access method, when alerted with power ringing, the utility controller shall go off-hook and become active.

With the COSU access method, the utility controller may initiate calls with the telephone network. Multiple calls may be placed during a single off-hook session.

With the direct dial access method, the utility controller may initiate calls with the telephone network. Only one call may be placed during a single off-hook session.

The utility controller shall go on-hook and become inactive:

- a) By its own initiative (end of data, error recovery, etc.);
- b) From a loss of carrier;
- c) From a disconnect signal in the data stream; and
- d) A maximum of 600 ms after the start of a disconnect signal (800 ms open) from the telephone network.

At the end of the 800 ms disconnect signal, the telephone network (switch) must look for an off-hook signal from the utility controller. If an off-hook signal exists, the telephone network (switch) must deliver a dial tone to the utility controller line.

5.2.4 Application

With the COSU access method, the utility controller must be connected to the telephone network (COSU) or network gateway. The utility controller will not have a through connection to the end user's line and will not supervise the utility telemetry trunk (UTT).

With the direct dial access method, the utility controller is directly connected to the end user's line.

End user TIU communications elements are stored in the utility controller database. For the COSU access method, examples of these elements are as follows: