



International
Standard

ISO 16140-7

**Microbiology of the food chain —
Method validation —**

**Part 7:
Protocol for the validation
of identification methods of
microorganisms**

*Microbiologie de la chaîne alimentaire — Validation des
méthodes —*

*Partie 7: Protocole pour la validation de méthodes
d'identification des micro-organismes*

**First edition
2024-11**



COPYRIGHT PROTECTED DOCUMENT

© ISO 2024

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 General principles for the validation of identification methods of microorganisms	4
5 Strains	4
6 Performance characteristics of an identification method	5
6.1 General	5
6.2 Description of the concept and limitation(s) of the identification method	5
6.3 Identification reliability of the identification method	6
6.3.1 Number of strains to be tested	6
6.3.2 Selection of the strains	7
6.3.3 Testing of the strains	7
6.3.4 Expression and interpretation of results	8
6.4 Evaluation	9
7 Interlaboratory study	10
7.1 General	10
7.2 Data sets to be obtained	10
7.3 Protocol	11
7.4 Expression of results	11
7.5 Interpretation and evaluation	12
Annex A (informative) Guidelines for the validation of methods for the identification of microorganisms in ecosystems	14
Annex B (normative) Points to be considered when selecting strains for an identification reliability study	21
Annex C (informative) Expression, interpretation and evaluation of results	22
Annex D (informative) Illustrations on the validation of methods for the identification of microorganisms in ecosystems	30
Bibliography	35

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO document should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

ISO draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at www.iso.org/patents. ISO shall not be held responsible for identifying any or all such patent rights.

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 34, *Food products*, Subcommittee SC 9, *Microbiology*, in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/TC 463, *Microbiology of the food chain*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

A list of all parts in the ISO 16140 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

0.1 The ISO 16140 series

The ISO 16140 series has been expanded in response to the need for various ways to validate or verify test methods. It is the successor to ISO 16140:2003. The ISO 16140 series consists of several parts with the general title, *Microbiology of the food chain — Method validation*:

- *Part 1: Vocabulary;*
- *Part 2: Protocol for the validation of alternative (proprietary) methods against a reference method;*
- *Part 3: Protocol for the verification of reference methods and validated alternative methods in a single laboratory;*
- *Part 4: Protocol for method validation in a single laboratory;*
- *Part 5: Protocol for factorial interlaboratory validation for non-proprietary methods;*
- *Part 6: Protocol for the validation of alternative (proprietary) methods for microbiological confirmation and typing procedures;*
- *Part 7: Protocol for the validation of identification methods of microorganisms.*

ISO 17468 is a closely linked International Standard, which establishes technical rules for the development and validation of standardized methods.

In general, two stages are needed before a method can be used in a laboratory.

- The first stage is the validation of the method. Validation is conducted using a study in a single laboratory followed by an interlaboratory study (see ISO 16140-2, ISO 16140-5, ISO 16140-6 and as described in this document). In the case when a method is validated within one laboratory (see ISO 16140-4), no interlaboratory study is conducted.
- The second stage is method verification, where a laboratory demonstrates that it can satisfactorily perform a validated method. This is described in ISO 16140-3. Verification is only applicable to methods that have been validated using an interlaboratory study.

In general, two types of methods are distinguished: reference methods and alternative methods.

A reference method is defined in ISO 16140-1:2016, 2.59, as an “internationally recognized and widely accepted method”. The note to entry clarifies that “these are ISO standards and standards jointly published by ISO and CEN or other regional/national standards of equivalent standing”.

In the ISO 16140 series, reference methods include standardized reference (ISO and CEN) methods as defined in ISO 17468:2023, 3.7, as a “reference method described in a standard”.

An alternative method (method submitted for validation) is defined in ISO 16140-1:2016, 2.4, as a “method of analysis that detects or quantifies, for a given category of products, the same analyte as is detected or quantified using the corresponding reference method”. The note to entry clarifies that: “The method can be proprietary. The term ‘alternative’ is used to refer to the entire ‘test procedure and reaction system’. This term includes all ingredients, whether material or otherwise, required for implementing the method”.

ISO 16140-4 addresses validation within a single laboratory. The results are therefore only valid for the laboratory that conducted the study. In this case, verification (as described in ISO 16140-3) is not applicable. ISO 16140-5 describes protocols for non-proprietary methods where a more rapid validation is required or when the method to be validated is highly specialized and the number of participating laboratories required by ISO 16140-2 cannot be reached. ISO 16140-4 and ISO 16140-5 can be used for validation against a reference method. ISO 16140-4 (regarding qualitative and quantitative methods) and ISO 16140-5 (regarding quantitative methods only) can also be used for validation without a reference method.

The flow chart in [Figure 1](#) gives an overview of the links between the different parts mentioned above. It also guides the user in selecting the right part of the ISO 16140 series, taking into account the purpose of the study and the remarks given above.

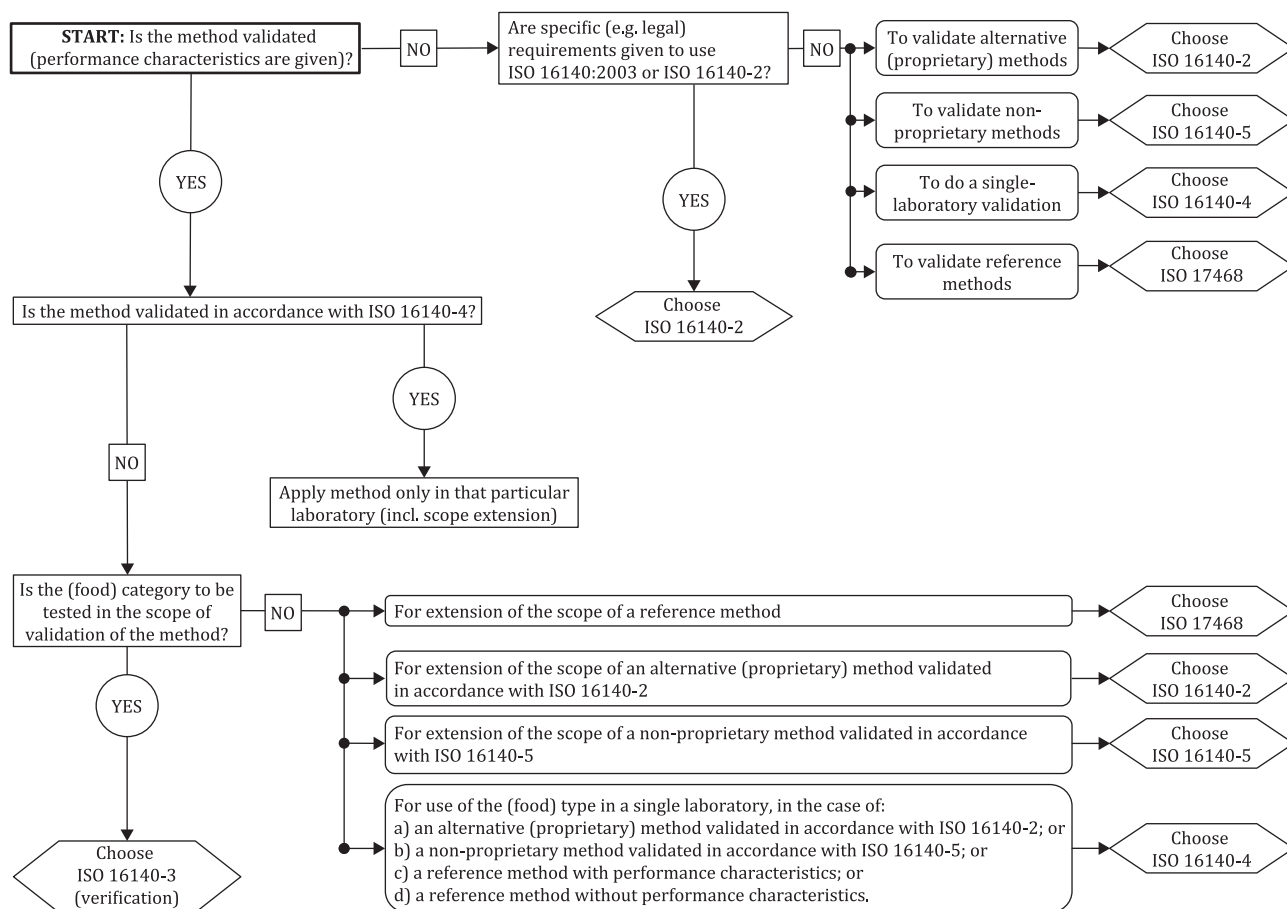


Figure 1 — Flow chart for application of ISO 16140-2 to ISO 16140-5

NOTE 1 In this document, the words “category”, “type” and/or “item” are sometimes combined with “(food)” to improve readability. However, the word “(food)” is interchangeable with “(feed)” and other areas of the food chain as mentioned in [Clause 1](#).

ISO 16140-6 and this document (ISO 16140-7) are somewhat different from the other parts in the ISO 16140 series in that they relate to very specific situations.

ISO 16140-6 is restricted to the confirmation procedure of a method to be validated [e.g. the biochemical confirmation of *Enterobacteriaceae* (see ISO 21528-2)]. The confirmation procedure advances a suspected (presumptive) result to a confirmed positive result. The validation of alternative typing techniques (e.g. serotyping of *Salmonella*) is also covered by ISO 16140-6. The validation study in ISO 16140-6 clearly specifies the selective agar(s) from which strains can be confirmed using the alternative confirmation method. If successfully validated, the alternative confirmation method can only be used if strains are recovered on an agar that was used and was shown to be acceptable within the validation study. [Figure 2](#) shows the possibilities where an alternative confirmation method validated in accordance with ISO 16140-6 can be applied (see text in the boxes).

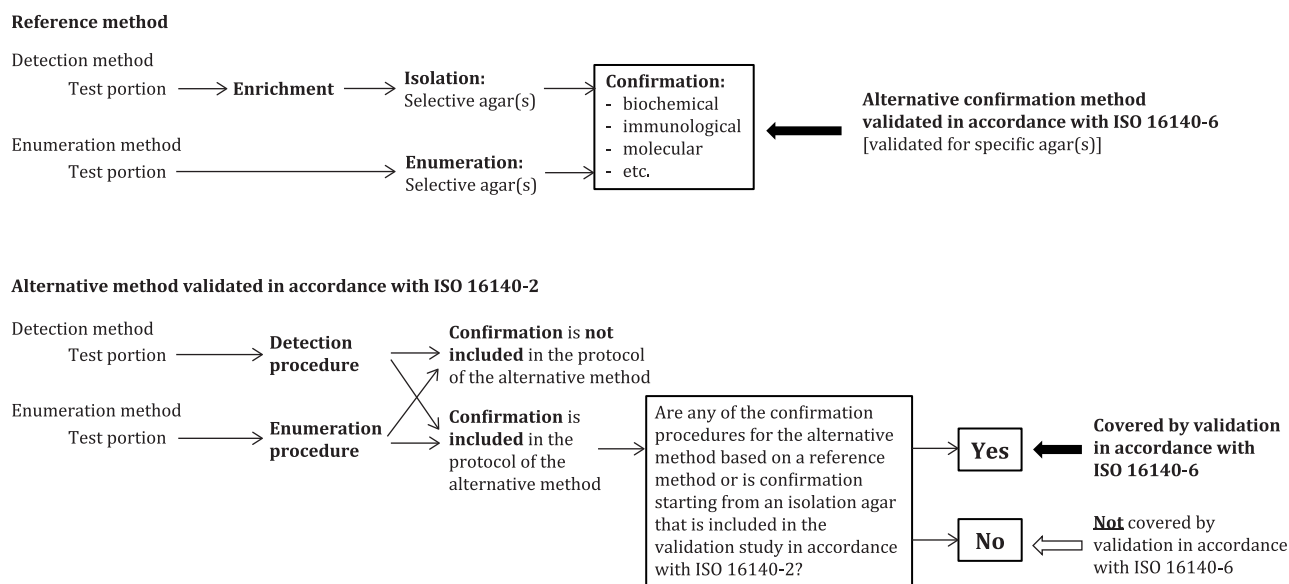


Figure 2 — Use of validated alternative confirmation methods (see ISO 16140-6)

EXAMPLE 1 An example application of a validated alternative confirmation method is as follows.

An alternative confirmation method based on ELISA has been validated to replace the biochemical confirmation for *Salmonella* as described in ISO 6579-1. In the validation study, XLD (mandatory agar in accordance with ISO 6579-1) plus BGA and a specified chromogenic agar (two optional agars for second plating in accordance with ISO 6579-1) were used as the agars to start the confirmation. The validated confirmation method can be used to replace the biochemical confirmation under the following conditions:

- by laboratories using ISO 6579-1; or
- by laboratories using an ISO 16140-2 validated alternative method that refers to ISO 6579-1 for confirmation; or
- by laboratories using an ISO 16140-2 validated alternative method that starts the confirmation from XLD and/or BGA agar and/or the specified chromogenic agar.

The validated confirmation method cannot be used under the following conditions:

- by laboratories using an ISO 16140-2 validated alternative method that refers only to agars other than those included in the validation to start the confirmation (e.g. Hektoen agar and SS agar only); or
- by laboratories using an ISO 16140-2 validated alternative method that refers only to a confirmation procedure that does not require isolation on agar.

This document (ISO 16140-7) addresses the validation of identification procedures (e.g. molecular identification using multiplex PCR or DNA sequencing or mass spectrometry). This document differs from the other parts in the ISO 16140 series, as it is intended for microbial identification for which there is no reference method and, therefore, it is not possible to run a method comparison study. The validation study in this document specifies the identification method principle, the identification database and algorithm when appropriate, and the agar(s) from which strains can be identified. If properly characterized and successfully validated, the identification method can only be validly used on strains recovered on the agars covered and shown to have been acceptable within the validation study.

NOTE 2 Whole-genome sequencing (WGS) in accordance with ISO 23418 will eventually be a reference method for all microorganisms, but the implementation of this technique is still at an early stage. Therefore, the use of WGS cannot currently be requested as a reference method for a large panel of strains.

Figure 3 shows the possibilities where an alternative confirmation method validated in accordance with ISO 16140-6 and an alternative identification method validated in accordance with this document can be applied within a reference method or an ISO 16140-2 validated detection or enumeration method. The result provided by the ISO 16140-7 validated method can be considered as additional information on the identity of the tested colony(ies); this result cannot be taken as a confirmation result. When there is a discrepancy

between the results of the ISO 16140-6 validated method and the ISO 16140-7 validated method, a root cause analysis is conducted. An ISO 16140-7 validated method can also be used to identify colonies within methods that do not require a confirmation step.

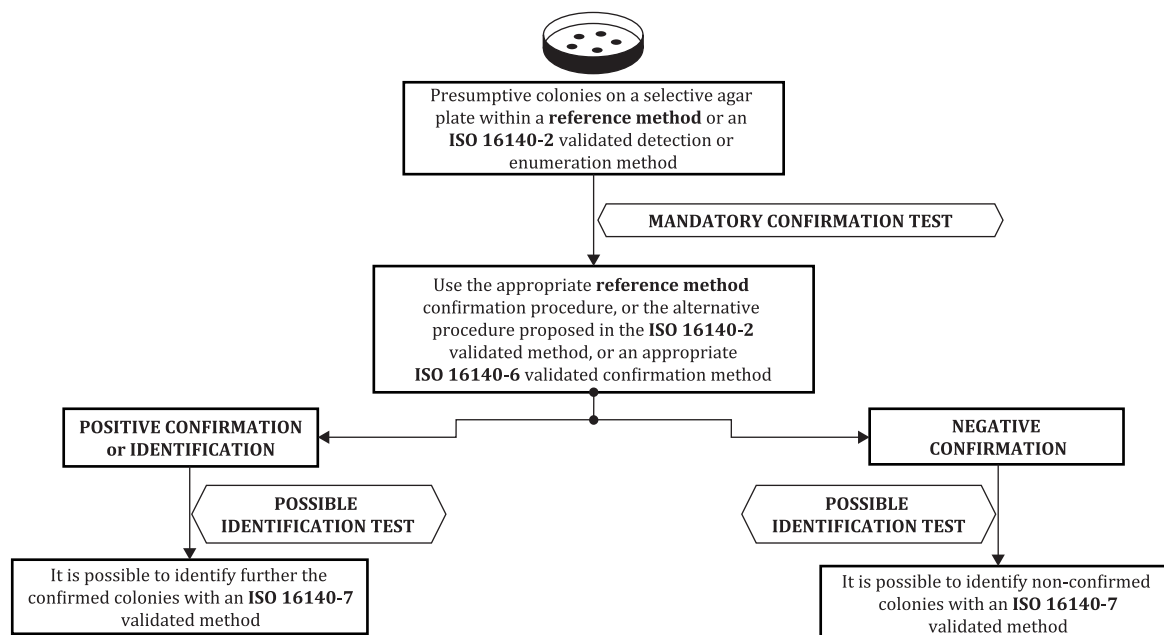


Figure 3 — Flow chart for the application of ISO 16140-6 and this document for the confirmation and identification of colonies within a reference method or an ISO 16140-2 validated detection or enumeration method

If the identification method is also validated in accordance with ISO 16140-6, the same method can be used for both confirmation and identification.

When a confirmation method is used, it is possible to apply an identification method validated in accordance with this document for further identification.

EXAMPLE 2 An alternative confirmation method of *Campylobacter* genus can be validated in accordance with ISO 16140-6 and compared to the mandatory confirmation procedure at the genus level described in ISO 10272-1. The identification at the *Campylobacter* species level is optional in ISO 10272-1 and ISO 10272-2 and is therefore not mandatory. In this instance, an identification method at the *Campylobacter* species level can be validated in accordance with this document. If the method is validated by ISO 16140-6 and this document, it can be used for both confirmation and identification purposes.

0.2 Validation and verification of identification methods of microorganisms

The procedure described in this document is intended for validation of identification methods of microorganisms. This procedure comprises two parts: a performance characteristics study and an interlaboratory study.

The procedure for validation of identification methods of microorganisms in a single laboratory is described in ISO 16140-4. The procedure for verification of identification methods of microorganisms in a single laboratory is described in ISO 16140-3.

Microbiology of the food chain — Method validation —

Part 7: Protocol for the validation of identification methods of microorganisms

1 Scope

This document specifies the general principle and the technical protocol for the validation of identification methods of microorganisms for microbiology in the food chain. As there is no reference method, no method comparison study can be run. Therefore, this document provides a protocol to evaluate the performance characteristics and validate the method workflow using well-defined strains. When required, an additional identification method can be used.

This document is applicable to the validation of identification methods of microorganisms that are used for the analysis of isolated colonies from:

- products intended for human consumption;
- products for feeding animals;
- environmental samples in the area of food and feed production and handling;
- samples from the primary production stage.

Identification methods only validated in accordance with this document cannot be used instead of confirmation described in:

- the reference method;
- an alternative method validated in accordance with ISO 16140-2;
- an alternative method validated in accordance with ISO 16140-6.

In these instances, the identification method is validated in accordance with ISO 16140-6 method that is used as a confirmation method.

This document is applicable to bacteria and fungi. Some clauses can be applicable to other (micro)organisms, which can be determined on a case-by-case basis.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 16140-1, *Microbiology of the food chain — Method validation — Part 1: Vocabulary*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 16140-1 and the following apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

3.1 **acceptability limit**

AL
maximum acceptable proportion of deviations between the reference identities (or if not known, the accepted reference values) of the strains or specimens and the corresponding identification results obtained when applying the operating procedure of the candidate identification method

Note 1 to entry: In the context of this document, the reference value can be the assigned identity of the strain.

3.2 **agreement**

identification agreement
method under validation study provides the same identification result as the assigned, i.e. original, identification of the tested strain

3.3 **assigned identity**

result of the microorganism identification displaying generally accepted molecular and/or biochemical characteristics

EXAMPLE Bergey's Manual of Systematics of Archaea and Bacteria^[13].

3.4 **comparison algorithm**

defined calculation rules used to compare the profile of the analysed strain to the database

3.5 **confirmation procedure**

confirmation test
procedure or test which is carried out to verify a presumptive result

Note 1 to entry: Not all methods have a confirmation procedure

Note 2 to entry: A confirmation test can provide a positive or negative result, without yielding the identity of the analyte.

[SOURCE: ISO 16140-1:2016, 2.17, modified — Note 2 has been included.]

3.6 **database**

library
collection of data categories and concept entry structure of an identification database

Note 1 to entry: An identification database usually gathers the phenotypic or molecular data information of several strains from the same species or genus.

Note 2 to entry: Some identification methods can have a restricted scope and do not imply a database (e.g. multiplex PCR assay).

3.7 **deviation**

identification deviation
method under validation study does not provide the same identification result as the assigned, i.e. original, identification of the tested strain

3.8

group

group of microbial ecosystems

specimens processed in a similar way, with similar intrinsic characteristics and a similar microbial ecology

EXAMPLE Enrichment broths.

3.9

homology

score

identity between the profile of the analysed strain and the entry(ies) in the database

Note 1 to entry: This is normally measured as % or with score value(s).

Note 2 to entry: For select identification methods (e.g. microarray), a homology score may not be obtained.

3.10

identification method

method submitted for validation

method of analysis that provides the name (identity) of the microorganism (e.g. species or higher taxonomy ranking level)

Note 1 to entry: The method can be non-proprietary or proprietary.

Note 2 to entry: The methods can be based on various principles (e.g. phenotypic and molecular principles).

Note 3 to entry: The identification of microorganisms can help for example in determining whether it is a safety or spoilage concern, or is a specific technological or probiotic strain, or is likely to be resistant to an inactivation treatment.

3.11

identification procedure

identification test

procedure or test yielding the identity of the analyte (e.g. species or higher taxonomy ranking level)

3.12

level of detection

LOD_x

relative concentration of the measured analyte in proportion to the total count of the specimen, obtained by a given measurement procedure, for which the probability of detection is x

EXAMPLE LOD_{50} is the level of detection for which 50 % of tests give a positive result.

[SOURCE: ISO 16140-1:2016, 2.35, modified — In the definition, “relative” and “in proportion to the total count of the specimen” have been added and the Note 1 to entry has been deleted.]

3.13

profile

set of characteristics that identify or are used to identify a strain

Note 1 to entry: The profile can be phenotypic (e.g. biochemical or serological) and/or molecular (e.g. DNA fingerprint, DNA sequence or mass spectra).

3.14

reliability

identification reliability

closeness of agreement between an identification result and the assigned identity of the tested strain

Note 1 to entry: The concept “identification reliability” is related to the identity of the analyte, i.e. genus or/and species names(s).

Note 2 to entry: “Identification reliability” is sometimes understood as closeness of agreement with the identification result that are being attributed to the identity of the strain given by another identification method.

3.15**risk of non-identification**

ratio of the probability of getting no identification result within a specified set of strains included in the scope of validation

Note 1 to entry: This does not apply to misidentification.

3.16**scope of validation**

database content and version, culture media or group of microbial ecosystems and comparison algorithm for which a validated method for the identification of microorganisms can be used satisfactorily

[SOURCE: ISO 16140-1:2016, 2.70 modified — In the definition, “analytes, matrices, and concentrations” has been replaced by “database content and version, culture media or group of microbial ecosystems and comparison algorithm”.]

4 General principles for the validation of identification methods of microorganisms

The validation protocol comprises two phases:

- a performance characteristics study;
- an interlaboratory study.

NOTE 1 For proprietary methods, the validation study is conducted by an organizing laboratory (see ISO 16140-1:2016, 2.45).

NOTE 2 It is possible, if relevant, to include inclusivity or exclusivity data obtained in an ISO 16140-2 or an ISO 16140-6 validation study into a study related to this document.

NOTE 3 As there is no reference identification method, there is no method comparison study.

The technical rules for performing the method performance characteristics study and the interlaboratory study are given in [Clauses 6](#) and [7](#). An extended set of strains from a non-selective agar or a selective agar when appropriate (e.g. yeasts and moulds) will be tested for both parts.

Where appropriate, the validation protocol shall also specify the selective media from which strains can be identified using the identification method. A specified number of strains shall be tested.

NOTE 4 The term “agar” is often referred to as “solid culture medium”.

NOTE 5 Other applications of identification methods are possible (e.g. identification of microorganisms in an ecosystem), see [Annex A](#) for further information.

NOTE 6 The identification procedure can be ensured by the collaboration of multiple laboratories. For instance, a first laboratory can isolate the strains and run the sample preparation such as DNA extraction and sequencing; the generated data can be analysed by comparison to the database held and managed by a second laboratory. In such a case, during the interlaboratory study, multiple collaborators will be involved in the sample preparation and will send the results for analysis to the laboratory managing the identification data interpretation.

5 Strains

The pure strains used for determining the identification reliability of the method shall be well-characterized in line with the purpose of the validation study. When necessary, the identification information provided by a second identification is used to evaluate the discrepancies between the results of the tested identification method and the assigned identity of the strain.

NOTE 1 National, regional or international reference laboratories can be contacted during such investigations.

NOTE 2 Well-characterized strains are strains that can be obtained from national/international culture collections, or ones that have been obtained locally and have been previously identified and given the same identity using usually two or more identification methods that are based on dissimilar principles.

NOTE 3 When appropriate, select strains with available WGS data in accordance with ISO 23418.

6 Performance characteristics of an identification method

6.1 General

The performance characteristics study is the part of the validation that is performed in one laboratory. It consists of a description of the concept and limitation(s) of the identification method, and an identification reliability study of the method. The results are then compared to those of the assigned identities of the tested set of strains.

6.2 Description of the concept and limitation(s) of the identification method

The method characteristics described in [Table 1](#) shall be carefully described in the method protocol (e.g. standard operation procedure, instructions for use) to enable proper use of the identification method by the end-user.

Table 1 — Essential components of the performance characteristics study

Characteristics	Detailed information
Scope of validation	Database description including name, version and content Culture media Microorganism name or type (e.g. bacteria, yeast, moulds, lactic acid bacteria, <i>Listeriaceae</i>) Comparison algorithm version
Identification method principle	Description of the strain profile/sequence and instrument signal acquisition used for identification of microorganisms
Database content	List of the genera and species in the database version used in the validation study
Concept of the database	Description of the types of signal profiles in the database, e.g. one unique profile selected as a representative for various strains of the same species or several signal profiles of various strains of the same species
Strains per species and genera in database	Number of strains per species and genera A minimum of 5 strains is required to claim a species in the database content
Limitations	List of the closely related species that are not differentiated by the identification method, size of the database
Comparison algorithm	Calculation of the result reporting, e.g. comparison of the instrument signal profile of the analysed strain to each single profile in the database or comparison of the profile of the analysed strain to unique average profiles for each species of the database.
Result reporting	Description of the homology concept used to assess the identification results with high confidence or low confidence
Strain preparation and troubleshooting	Description of the strain preparation and method workflow, particularly when obtaining homology result of low confidence or when no identification result is generated

In some very specific cases, the minimum number of strains per species in the database can be lower than the required 5 strains due to the lack of available strains. There should be a disclaimer in the database content for strains that do not meet the minimum requirement.

If the identification method does not imply a database (e.g. multiplex PCR assay), the description of the concept and limitation(s) of the identification method should be restricted to the scope of validation, the identification method principle, the limitations, the result reporting, the strain preparation and troubleshooting.

6.3 Identification reliability of the identification method

6.3.1 Number of strains to be tested

The set of strains to be tested depends on the database content and the scope of the validation. Select, as much as possible, one strain per species to ensure that at least 25 % of genera and 10 % of species contained in the database are tested. However, a minimum and a maximum number of strains to be tested has been specified at, respectively, 250 strains and 1 000 strains. For restricted database content (e.g. 25 genera and 200 species), test all the genera and species.

[Figure 4](#) provides examples of how to determine the appropriate number of strains to be tested.

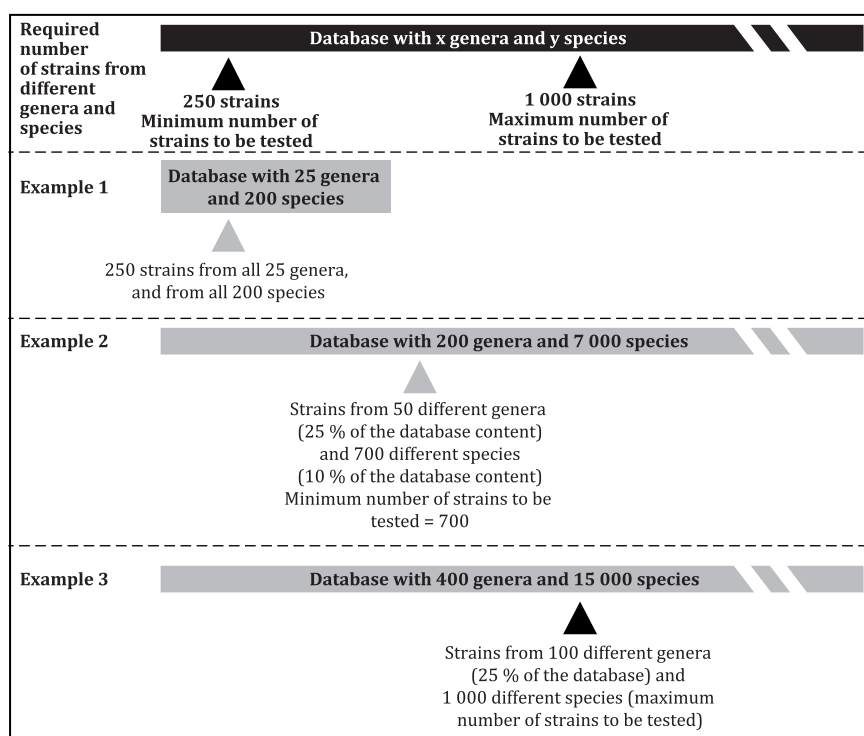


Figure 4 — Examples on how to determine the number of strains to be tested

Pure cultures from a non-selective agar of all selected strains shall be tested by the identification method.

NOTE 1 Non-selective agars (e.g. TSA) enable the recovery of a broad range of microorganisms and can favour the recovery of some specified groups of microorganisms. For microorganisms, for which non-selective agars are not known or are not supported by corresponding standardized reference methods for the isolation of the respective microorganism, only selective agars can be used instead.

If the scope of the validation study also includes selective agars, refer to [Table 2](#) for the number of relevant genera and species to be tested for each selective agar included in the scope.

NOTE 2 Selective agars can enable the recovery of microorganisms from specific clades, (i) family, (ii) genus or group of species (e.g. *Bacillus cereus* group). In this document, “group of species” is substituted with “genus” to improve readability. However, the word “genus” is interchangeable with “group of species”.