
**Fine ceramics (advanced ceramics,
advanced technical ceramics) — Test
method for flexural strength of monolithic
ceramics at elevated temperature**

*Céramiques techniques — Méthode d'essai de résistance à la flexion
des céramiques monolithiques à température élevée*



PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

© ISO 2003

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

	Page
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	3
5 Apparatus	3
5.1 Testing machine	3
5.2 Heating device	3
5.3 Temperature measuring and indicating instruments	4
5.4 Testing fixture	5
5.5 Micrometer	9
6 Test pieces	9
6.1 Test piece size	9
6.2 Test piece preparation	10
7 Procedure	10
8 Calculation	13
8.1 Standard formula for the flexural strength in four-point flexure	13
8.2 Standard formula for the flexural strength in three-point flexure	14
8.3 Corrections for chamfer size	14
8.4 Corrections for thermal expansion	14
8.5 Mean strength and standard deviation	15
9 Accuracy and precision	15
10 Test report	15
11 Strength scaling factors	16
Annex A (informative) General information	17
Annex B (normative) Chamfer correction factors	18
Annex C (normative) Corrections for thermal expansion	21
Annex D (informative) Weibull scaling factors	23
Annex E (informative) VAMAS round robin	25
Bibliography	26

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 17565 was prepared by Technical Committee ISO/TC 206, *Fine ceramics*.

Document Sharing Hub

Fine ceramics (advanced ceramics, advanced technical ceramics) — Test method for flexural strength of monolithic ceramics at elevated temperature

1 Scope

This International Standard describes the method of test for determining the flexural strength of monolithic fine ceramics and whisker- or particulate-reinforced ceramic composites at elevated temperature. Flexural strength is one measure of the uniaxial strength of fine ceramics. This test method may be used for materials development, quality control, characterization and design data generation purposes.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3611:1978, *Micrometer callipers for external measurement*

ISO 7500-1:—¹⁾, *Metallic materials — Verification of static uniaxial testing machines — Part 1: Tension/compression testing machines — Verification and calibration of the force-measuring system*

ISO 14704:2000, *Fine ceramics (advanced ceramics, advanced technical ceramics) — Test method for flexural strength of monolithic ceramics at room temperature*

IEC 60584-1:1995, *Thermocouples — Part 1: Reference tables*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

flexural strength

maximum nominal stress at fracture of a specified elastic beam loaded in bending

3.2


four-point flexure

configuration of flexural strength testing where a test piece is equally loaded by two bearings symmetrically located between two support bearings


See Figure 1.

NOTE The bearings may be cylindrical rollers or cylindrical bearings.


1) To be published. (Revision of ISO 7500-1:1999)

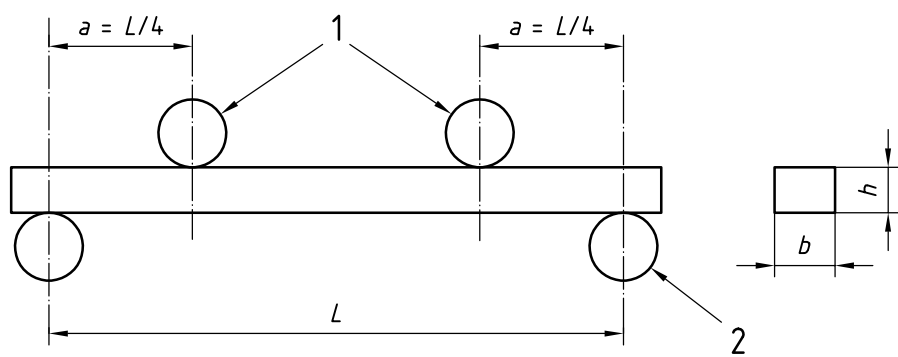

a) Four-point-1/4 point flexure

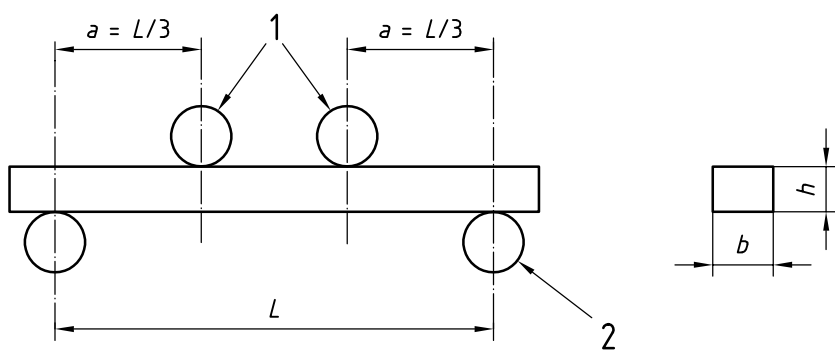

b) Four-point-1/3 point flexure

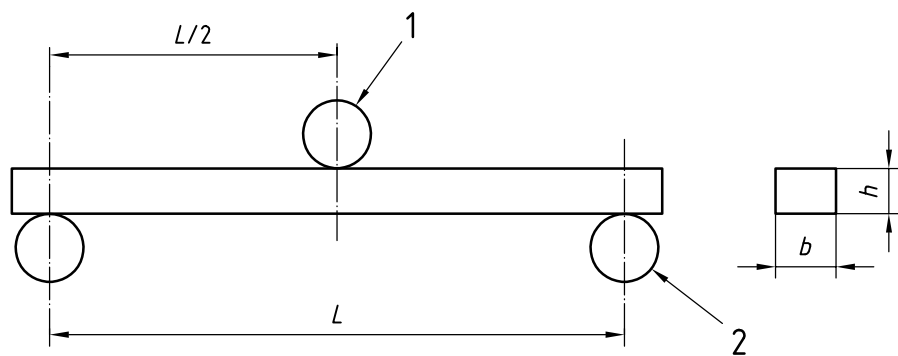

c) Three-point flexure

- Key**
- 1 loading bearings
 - 2 support bearing

Figure 1 — Flexural test configurations

3.3
four-point-1/4 point flexure

specific configuration of four-point flexural strength testing where the inner bearings are situated one quarter of the support span away from the two outer bearings

See Figure 1 a).

3.4**four-point-1/3 point flexure**

specific configuration of four-point flexural strength testing where the inner bearings are situated one third of the support span away from the two outer bearings

See Figure 1 b).

3.5**three-point flexure**

configuration of flexural strength testing where a test piece is loaded at a location midway between two outer bearings

See Figure 1 c).

NOTE Four-point flexure is usually preferred since a larger amount of material is exposed to the maximum stress. See Bibliography for more information.

4 Principle

A beam test piece with a rectangular cross section is loaded in flexure until fracture. The load at fracture, the test fixture and test piece dimensions are used to compute the flexural strength, which is a measure of the uniaxial tensile strength of a ceramic. The material is assumed to be isotropic and linearly-elastic. Testing is performed at elevated temperature in air or inert atmosphere. Load is monitored versus displacement or time in order to confirm that the beam test piece fractured under elastic conditions. This International Standard is an elevated-temperature adaptation of ISO 14704. See Annex A for additional information on this test method.

5 Apparatus**5.1 Testing machine**

A suitable testing machine capable of applying a uniform crosshead speed shall be used. The testing machine shall be in accordance with ISO 7500-1:— Class 1 with an accuracy of 1 % of indicated load at fracture.

5.2 Heating device**5.2.1 General**

The furnace shall be capable of heating the test fixture and test piece as well as maintaining a uniform and constant temperature during the strength test. The furnace may have an air, inert gas or vacuum environment, as required. If an inert gas or vacuum chamber is used, and it is necessary to transmit the load through a seal, bellows or a fitting, it shall be verified that load losses or errors are less than 1 % of the expected fracture loads. The furnace may be designed so that test pieces are loaded into either hot or cold furnaces.

5.2.2 Test piece temperature stability

The furnace shall be controlled by a device for maintaining a constant temperature within $\pm 2^\circ\text{C}$ or better within the working space of the furnace, during the time that the test piece is loaded to fracture.

5.2.3 Test piece temperature uniformity

The furnace shall be capable of maintaining the test piece temperature uniform. It shall previously be determined that the temperature of the test piece shall not vary more than 10°C over its length after a 15 min hold time at the required test temperature.

5.2.4 Furnace heating rate

The furnace control device shall also be capable of controlling the heating rates of the furnace and preventing temperature overshoots.

5.2.5 Furnace stability

The time for the system to reach thermal equilibrium at test temperature shall be determined for the test temperature to be used.

5.3 Temperature measuring and indicating instruments

5.3.1 General

Thermocouple temperature measuring equipment shall have a resolution of at least 1 °C and an accuracy of 5 °C or better. Optical pyrometers, if used, shall have a resolution of at least 5 °C and an accuracy of 5 °C or better.

NOTE 1 Resolution should not be confused with accuracy. Beware of instruments that have a resolution (read out) of 1 °C, but have an accuracy of only 10 °C; e.g., an instrument with a 1 % accuracy would only be accurate to ± 12 °C at 1 200 °C.

NOTE 2 Thermocouple temperature measuring instruments typically approximate the temperature-electromotive force (EMF) tables, but with a few degrees error.

5.3.2 Thermocouples

Thermocouples in accordance with IEC 60584-1 shall be used. The thermocouples shall exhibit low thermal inertia (the diameter of the wires shall not be greater than 0,5 mm). The thermocouples shall have a sufficient length within the furnace (with respect to heat conduction along the wires). The measuring thermocouple tip shall be as close as possible to or contacting the test piece.

NOTE 1 In some furnaces, a control thermocouple may be installed at a location within the furnace which is convenient for furnace control and a second measuring thermocouple may be in close proximity to the test piece.

NOTE 2 The thermocouple should not contact the test piece if there is a chance the test piece will be misaligned.

NOTE 3 The thermocouple should not contact the test piece if it will chemically react with the test piece.

5.3.3 Verification of the thermocouple temperature measuring system

Thermocouples shall be checked periodically since calibration may drift with usage or contamination.

5.3.4 Radiation pyrometers

Radiation pyrometers (thermometers) may be used in instances wherein suitable thermocouples are not available, particularly at temperatures above 1 600 °C. Pyrometers may either be of the disappearing filament type or an automatic type. Pyrometers may either be spectral (operate over a narrow wavelength band), dual wavelength (operate over two narrow wavelength bands) or total (integrate or average over all wavelengths). Radiation pyrometry requires special care in order to obtain accurate and precise results. Ensure that blackbody conditions are obtained, or correct the temperature for the actual emissivity of the test piece in its environment. The pyrometer should view the test piece at right angles to one of the four long surfaces. The target size (or viewed area) of the pyrometer shall be less than 3 mm in diameter. Corrections for radiation absorption or reflectance may be necessary if the furnace has a window. The window shall be sufficiently large such that the radiation emanating from the window completely fills the objective lens of the radiation thermometer, but the window should not be so large as to cause appreciable heat loss or thermal gradients in the furnace.

NOTE See ASTM Standard Test Methods E 452, E 639, E 1256, and BS 1041, part 5 for additional information.

5.4 Testing fixture

5.4.1 General

Three- or four-point flexure configurations shall be used as illustrated in Figures 1 and 2. The four-point-1/4-point configuration is recommended. The fixtures shall either be semi-articulating or fully-articulating as specified in ISO 14704 depending upon the condition of the test pieces. If the test pieces meet the parallelism requirements of 6.1.1 and Figure 3, either a semi-articulating fixture or fully articulating fixture may be used. If the test pieces do not meet the parallelism requirements of 6.1.1 and Figure 3, a fully-articulating fixture shall be used.

NOTE 1 Machined test pieces normally have flat and parallel surfaces and semi-articulating fixtures are completely satisfactory. On the other hand, as-fired, heated treated or oxidized test pieces often do not meet the parallelism requirements. Twisting of the test piece can cause severe errors in the strength calculation, unless a fully-articulating fixture is used. The purpose of articulation is to ensure that the bearings have uniform and even contact with the test piece surface.

NOTE 2 A fully-articulating fixture has bearings or rollers that are free to roll to eliminate friction. The bearings articulate independently to match the test piece surface.

NOTE 3 A semi-articulating fixture has bearings or rollers that are free to roll to eliminate friction. The bearings articulate in pairs to match the test piece surface.

It is recognized that practical limitations may restrict the design of the test fixture, and oxidation effects may restrict its function. In such cases, alternatives may be employed, but deviations from the function specified above shall be reported in the report.

5.4.2 Bearings

Test pieces shall be loaded and supported by bearings. The bearings shall be cylindrical rollers. The bearing length shall be greater than or equal to 12 mm. The bearing diameter shall be approximately 1,5 times the test piece thickness, h . Diameters between 4,5 mm and 5,0 mm are recommended. The bearings shall have a smooth surface and shall have a diameter uniform to $\pm 0,015$ mm. All bearings shall be free to roll in order to eliminate friction, with the exception of the middle bearing in three point flexure (see Figure 2). For four-point flexure, the two inner bearings shall be free to roll *inwards*, and the two outer bearings shall be free to roll *outwards*. In three-point flexure, the two outer bearings shall be free to roll outwards, and the inner (middle) bearing should not roll.


NOTE 1 Friction can cause errors in the stress calculations. The rolling action in elevated temperature fixtures is usually accomplished by using cylindrical bearings which rest on a flat surface. The bearings are free to roll on the surface as shown in Figure 2.

NOTE 2 The bearing diameter is specified on the basis of competing requirements. The bearings should not be so large as to cause excessive change in the moment arm (" a " in Figure 1) as a test piece deflects which can create errors from contact-point tangency shift. On the other hand, the bearings should not be so small as to create excessive wedging or contact stresses in the test piece.

5.4.3 Four-point fixture — Semi-articulating


All four bearings shall be free to roll. The two inner bearings shall be parallel to each other to within 0,015 mm over their length (≥ 12 mm in accordance with 5.4.2). The two outer bearings shall be parallel to each other to within 0,015 mm over their length. The inner bearings shall be supported independently of the outer bearings. All four bearings shall rest uniformly and evenly across the test piece surface. The fixture shall be designed to apply equal loads to all four bearings.

NOTE The parallelism requirement may be met by control of the test fixture dimensions.

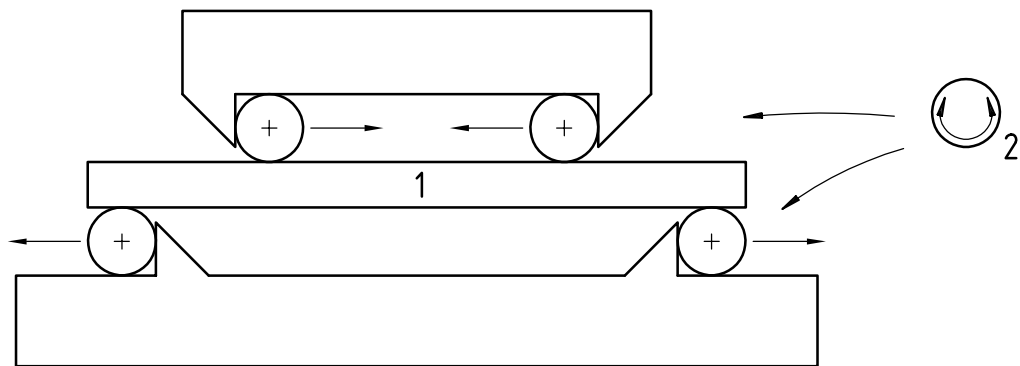

The four bearings shall be free to roll in four-point flexure

a) Four-point flexure

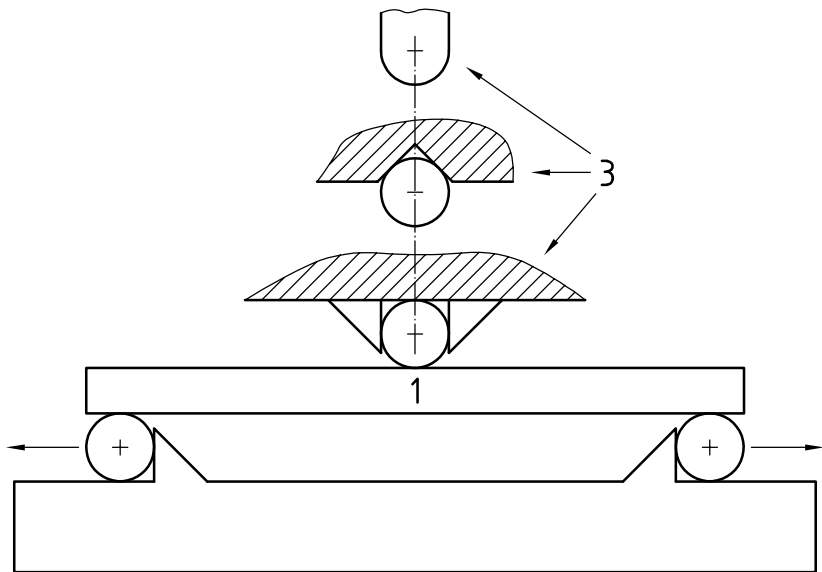

The two outer bearings are free to roll outwards in the three-point flexure, but the middle bearing shall be non-rolling

b) Three-point flexure

- Key**
- 1 test piece
 - 2 alternative rolling bearings
 - 3 alternatives

Figure 2 — Schematic of semi-articulating fixtures