PD IEC/TS 62622:2012

BSI Standards Publication

Nanotechnologies — Description, measurement and dimensional quality parameters of artificial gratings

NO COPYING WITHOUT BSI PERMISSION EXCEPT AS PERMITTED BY COPYRIGHT LAW

raising standards worldwide™

Full document details: PD IEC/TS 62622:2012

National foreword

This Published Document is the UK implementation of IEC/TS 62622:2012.

The UK participation in its preparation was entrusted to Technical Committee NTI/1, Nanotechnologies.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2013

Published by BSI Standards Limited 2013

ISBN 978 0 580 80384 0

ICS 07.030

Compliance with a British Standard cannot confer immunity from legal obligations.

This Published Document was published under the authority of the Standards Policy and Strategy Committee on 28 February 2013.

Amendments issued since publication

Amd. No.	Date	Text affected

Documents
Document Sharing Hub

Full document details: PD IEC/TS 62622:2012

IEC/TS 62622

Edition 1.0 2012-10

TECHNICAL SPECIFICATION

Nanotechnologies – Description, measurement and dimensional quality parameters of artificial gratings

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

PRICE CODE W

ICS 07.030

ISBN 978-2-83220-394-1

Warning! Make sure that you obtained this publication from an authorized distributor.

Documents
Document Sharing Hub

Full document details: PD IEC/TS 62622:2012

CONTENTS

FOREWORD 4
INTRODUCTION 6
1 Scope 7
2 Normative references 7
3 Terms and definitions 7
3.1 Basic terms 7
3.2 Grating terms 10
3.3 Grating types 11
3.4 Grating quality parameter terms 14
3.5 Measurement method categories for grating characterization 17
4 Symbols and abbreviated terms 18
5 Grating calibration and quality characterization methods 18
5.1 Overview 18
5.2 Global methods 18
5.3 Local methods 19
5.4 Hybrid methods 20
5.5 Comparison of methods 20
5.6 Other deviations of grating features 21
5.6.1 General 21
5.6.2 Out of axis deviations 21
5.6.3 Out of plane deviations 22
5.6.4 Other feature deviations 22
5.7 Filter algorithms for grating quality characterization 23
6 Reporting of grating characterization results 23
6.1 General 23
6.2 Grating specifications 24
6.3 Calibration procedure 24
6.4 Grating quality parameters 24
Annex A (informative) Background information and examples 25
Annex B (informative) Bravais lattices 34
Bibliography 38

Figure 1 – Example of a trapezoidal line feature on a substrate 8
Figure 2 – Examples of feature patterns 9
Figure 3 – Examples of 1D line gratings 12
Figure 4 – Example of 2D gratings 13
Figure A.1 – Result of a calibration of a 280 mm length encoder system which was used as a transfer standard in an international comparison [31] 27
Figure A.2 – Filtered (linear profile Spline filter with λ_C = 25 mm) results of Figure A.1 28
Figure A.3 – Calibration of a 1D grating by a metrological SEM 30
Figure A.4 – Calibration of pitch and straightness deviations on a 2D grating by a metrological SEM 31

AVA Documents
Document Sharing Hub
Full document details: PD IEC/TS 62622:2012

Figure A.5 – Results of an international comparison on a 2D grating by different participants and types of instruments 33
Figure B.1 – One-dimensional Bravais lattice 34
Figure B.2 – The five fundamental two-dimensional Bravais lattices illustrating the primitive vectors $\vec{a}$ and $\vec{b}$ and the angle φ between them 35
Figure B.3 – The 14 fundamental three-dimensional Bravais lattices 36

Table 1 – Comparison of different categories for grating characterization methods 21
Table A.1 – Grating quality parameters of the grating in Figures A.1 and A.2 28
Table A.2 – Grating quality parameters of the grating in Figure A.3 30
Table A.3 – Grating quality parameters of the grating in Figure A.4 32
Table B.1 – Bravais lattices volumes 37

Documents
Document Sharing Hub
Full document details: PD IEC/TS 62622:2012

INTERNATIONAL ELECTROTECHNICAL COMMISSION

NANOTECHNOLOGIES – DESCRIPTION, MEASUREMENT AND DIMENSIONAL QUALITY PARAMETERS OF ARTIFICIAL GRATINGS

FOREWORD

1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
6) All users should ensure that they have the latest edition of this publication.
7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

The main task of IEC technical committees is to prepare International Standards. In exceptional circumstances, a technical committee may propose the publication of a technical specification when

- the required support cannot be obtained for the publication of an International Standard, despite repeated efforts, or
- the subject is still under technical development or where, for any other reason, there is the future but no immediate possibility of an agreement on an International Standard.

Technical specifications are subject to review within three years of publication to decide whether they can be transformed into International Standards.

IEC 62622, which is a technical specification, has been prepared within the joint working group 2 of IEC technical committee 113 and ISO technical committee 229.

Documents
Document Sharing Hub
Full document details: PD IEC/TS 62622:2012

The text of this technical specification is based on the following documents:

Enquiry draft	Report on voting
113/133/DTS	113/143/RVC

Full information on the voting for the approval of this technical specification can be found in the report on voting indicated in the above table. In ISO, the standard has been approved by 16 member bodies out of 16 having cast a vote.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

The committee has decided that the contents of this publication will remain unchanged until the stability date indicated on the IEC web site under "http://webstore.iec.ch" in the data related to the specific publication. At this date, the publication will be

- transformed into an International Standard,
- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

A Bilingual version of this publication may be issued at a later date.

IMPORTANT – The “colour inside” logo on the cover page of this publication indicates that it contains colours which are considered to be useful for the correct understanding of its contents. Users should therefore print this publication using a colour printer.

Documents
Document Sharing Hub

Full document details: PD IEC/TS 62622:2012

INTRODUCTION

Artificial gratings play an important role in the manufacturing processes of small structures at the nanoscale as well as characterization of nano-objects.

For example, in high volume manufacturing of semiconductor integrated circuits by means of lithography techniques, grating patterns on the photomask and the silicon wafer are optically probed and the resulting optical signal is analyzed and used for relative alignment purposes of mask to wafer in the different lithographic production steps in the wafer-scanner production tools. In semiconductor manufacturing as well as in other manufacturing processes requiring high positioning accuracy at the nanoscale, often length or angular encoder systems based on artificial gratings are used to provide position feedback of moving axes. Another area of application for artificial gratings in nanotechnology is their use as calibration standards for high resolution microscopes, like scanning probe microscopes, scanning electron microscopes or transmission electron microscopes which are necessary tools for the characterization of nanoscale structures.

The quality of the artificial gratings used for position feedback generally influences the achievable accuracy of alignment systems or positioning systems in manufacturing tools. This also holds for the application of artificial gratings as standards for calibration of image magnification of high resolution microscopes, where the quality of the grating plays an important role in the achievable calibration uncertainty of the standard and thus for the attainable measurement uncertainty of the microscope.

This technical specification concentrates on specifying quality parameters, expressed in terms of deviations from nominal positions of grating features, and provides guidance on the application of different categories of measurement and evaluation methods to be used for calibration and characterization of artificial gratings

Documents
Document Sharing Hub
Full document details: PD IEC/TS 62622:2012

NANOTECHNOLOGIES – DESCRIPTION, MEASUREMENT AND DIMENSIONAL QUALITY PARAMETERS OF ARTIFICIAL GRATINGS

1 Scope

This technical specification specifies the generic terminology for the global and local quality parameters of artificial gratings, interpreted in terms of deviations from nominal positions of grating features, and provides guidance on the categorization of measurement and evaluation methods for their determination.

This specification is intended to facilitate communication among manufacturers, users and calibration laboratories dealing with the characterization of the dimensional quality parameters of artificial gratings used in nanotechnology.

This specification supports quality assurance in the production and use of artificial gratings in different areas of application in nanotechnology. Whilst the definitions and described methods are universal to a large variety of different gratings, the focus is on one-dimensional (1D) and two-dimensional (2D) gratings.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories*

ISO/TS 80004-1:2010, *Nanotechnologies – Vocabulary – Part 1: Core terms*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1 Basic terms

3.1.1
feature
region within a single continuous boundary, and referred to a reference plane, that has a defining physical property (parameter) that is distinct from the region outside the boundary

Documents
Document Sharing Hub

Full document details: PD IEC/TS 62622:2012

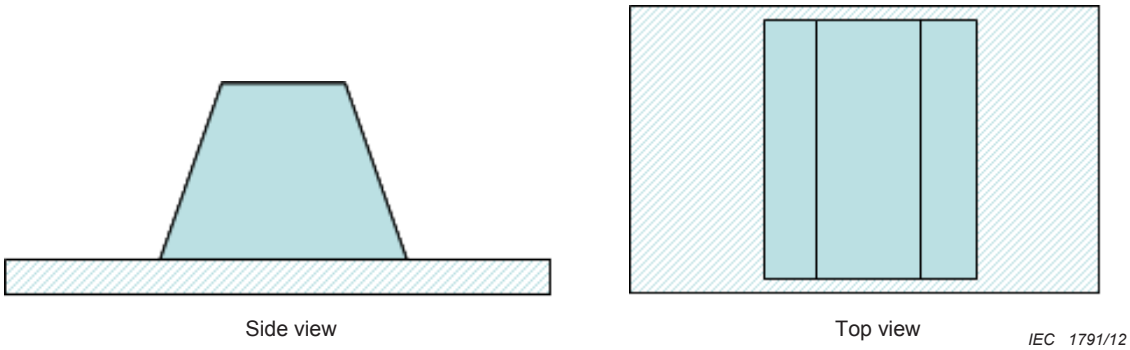

Figure 1 – Example of a trapezoidal line feature on a substrate

EXAMPLE In Figure 1 a feature with a trapezoidal cross-section on a substrate is shown.

Note 1 to entry: This definition is adapted from [1][1] (SEMI P35 (5.1.5 feature (lithographic)).

Note 2 to entry: In general, a feature is a three-dimensional object. It can also be a nano-object (defined in ISO/TS 80004-1:2010, 2.5). It can have different shape, e.g. it can be a dot, a line, a groove, etc. It might be symmetric or non–symmetric. It can have the same material properties as the substrate or different ones. It can be located on the surface of a substrate or within the substrate (sometimes called “buried feature”).

Note 3 to entry: In [2] the term ‘geometrical feature’ is generally defined as point, line or surface.

3.1.2
reference plane
user-defined plane approximating the surface of a substrate and containing a feature coordinate system

Note 1 to entry: This definition is adapted from [1].

3.1.3
feature coordinate system
coordinate system
Cartesian coordinate system defined by the reference plane as x-y plane, the x-axis defined by the main grating direction and the origin defined by a suitable, specified reference position

Note 1 to entry: Often, the position of a particular feature is chosen as the origin of the coordinate system, e.g. the first feature in a 1D grating, or the lower left feature in a 2D grating.

Note 2 to entry: In other cases, the origin can also be defined from an analysis of the positions of all features of interest, e.g. the mean value of all positions in the x-direction for a 1D grating. In the case of a 2D grating the origin can also be defined by a least squares regression fit over all measured x- and y-positions of all features of the 2D grating allowing translation of the origin and rotation of the whole 2D grating (so-called multi-point alignment). In these cases the origin of the feature coordinate system no longer corresponds to a particular feature.

Note 3 to entry: The origin can also be chosen as the position of a specified alignment feature or auxiliary feature within the reference plane.

Note 4 to entry: In case of angular gratings the feature coordinate system can favorably be defined as a polar coordinate system: r, φ or a cylindrical coordinate system: r, φ, z.

3.1.4
feature pattern
set of features, specified by number, type, and positions of features

[1] Numbers in square brackets refer to the Bibliography.

Documents
Document Sharing Hub
Full document details: PD IEC/TS 62622:2012

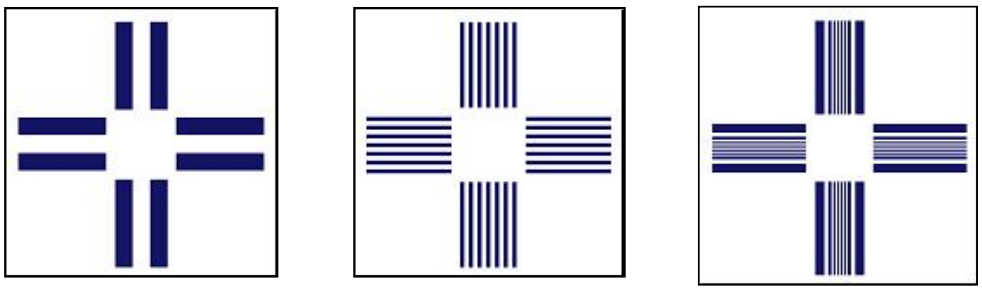

Figure 2 – Examples of feature patterns

EXAMPLE Figure 2 shows examples of different types of feature patterns.

Note 1 to entry: Different kinds of features can be arranged differently in a set to form feature patterns. These can be rather simple e.g. a single cross structure as a combination of two orthogonal line features, complex like, e.g. a double cross-structure or a line array or even more complex, e.g. irregularly spaced line features.

3.1.5
feature position
x_i, y_i, z_i
coordinates describing the position of a prescribed point of the ith feature of a number *N* of features projected onto the reference plane relative to a specified coordinate system

Note 1 to entry: For 1D gratings the x-positions of the features are primarily of interest assuming the direction of the grating, i.e. the direction in which the number of grating features per unit length is maximal, is the x-direction, whereas for 2D gratings their x- and y-positions are of interest. In both cases, their z-positions are usually of minor interest, assuming the *reference plane* is already well aligned to the axes of the measurement instrument.

Note 2 to entry: Depending on the chosen criterion for the feature position evaluation (see Note 3), the measured feature position is dependent on the interaction of the measurement instrument used with the feature characteristics, like its shape, size and material properties.

Note 3 to entry: The determination of the feature position is often based on the analysis of a microscopic image of the feature. The microscope image signals can be analyzed in different ways to determine the feature position. Mostly the centre position of the feature is of interest which can be determined, e.g. by calculation of the centroid or by determination of the mean value between the position of the left and the right edge of the feature.

Note 4 to entry: If only parts of the feature are of interest, e.g. the edge position of a line feature, the determination of the position of the respective edge(s) should be based only on the parts of the feature that are of interest.

Note 5 to entry: The above definition for the feature position can also be applied to a feature pattern.

Note 6 to entry: If angular gratings are analyzed, it is favorable to express the feature position in polar coordinates r, φ or in cylindrical ones r, φ, z.

3.1.6
distance between features
d
difference of the feature positions determined on equivalent or homologous feature characteristics in the direction of interest

Note 1 to entry: The distance *d* between two consecutive features, *i* and *i*-1, in the x-direction is:

$$d = \text{abs}\,(x_i - x_{i-1})$$

Note 2 to entry: The distance *d* between two consecutive features in the reference x,y plane generally is:

$$d = [(x_i - x_{i-1})^2 + (y_i - y_{i-1})^2]^{0,5}$$

Documents
Document Sharing Hub
Full document details: PD IEC/TS 62622:2012

Note 3 to entry: The distance d between two consecutive features at the positions x_i, y_i, z_i and x_{i-1}, y_{i-1} z_{i-1} in the general case is:

$$d = [(x_i - x_{i-1})^2 + (y_i - y_{i-1})^2 + (z_i - z_{i-1})^2]^{0,5}$$

Note 4 to entry: Usually the distance between features is of interest for the centre positions of the features. In some cases however the distance can also be of interest for positions on the feature edges.

3.2 Grating terms

3.2.1
grating
periodically spaced collection of identical features

Note 1 to entry: In [3], which provides a vocabulary of diffractive optics, a grating is defined as a "periodic spatial structure for optical use" (3.3.1.2). In this technical specification, gratings are not restricted to optical use only.

Note 2 to entry: Often gratings show a ratio of the distance between neighboring identical features to their size that is close to one. However, the definition is not restricted to these cases and also includes so-called sparse gratings and thus in principle line scales, too.

Note 3 to entry: Although this technical specification is primarily addressing periodic gratings, the definition of grating quality parameters should also be applicable to non-periodic gratings, like chirped gratings (3.3.5.2) as far as possible. Limitations might occur in particular for spatial filtering approaches of feature position data.

Note 4 to entry: Sometimes a grating can be divided into several sub-gratings having different features.

3.2.2
pitch
p
distance between neighboring features of a grating

Note 1 to entry: Often, the feature centre positions are used to determine the pitch. In some cases, however, also the distance between equivalent edges of a pair of features is used to determine the pitch values.

Note 2 to entry: This definition is in alignment with the definition for pitch as specified in [1] (5.1.14).

3.2.3
nominal pitch
p_{nom}
intended pitch value, indicated in the specification of a grating

3.2.4
number of grating features
N_f
result of a summation over all identical features of the grating in the direction of interest

Note 1 to entry: The number of grating features can be different in the different directions for 2D and three-dimensional (3D) gratings. The total number of features in 2D and 3D gratings is the product of the number of grating features along the 2 or 3 different directions (e.g. dots in the case of 1D features).

3.2.5
mean pitch
p_m
average pitch value determined over all identical features of the grating

Note 1 to entry: The mean pitch is not necessarily the arithmetic mean pitch, but any statistically characteristic pitch.

Note 2 to entry: If all feature positions of the grating are known, the mean pitch of a grating can be determined by a linear least squares regression fit of all measured feature positions $x_{i,\,m}$ to the nominal feature positions $x_{i,\,nom}$. If the uncertainties of the measured feature positions are equal, a standard linear regression fit can be applied. In case of a variation of the uncertainties u_{xi} of the measured feature positions $x_{i,\,m}$, a weighted linear regression fit should be applied, using the inverse variances as weights ($w_i = 1/(u_{xi})^2$). The resulting slope m of the regression line (yielding values for slope m and intercept b) can be used to calculate the mean pitch value $p_m = m \cdot p_{nom}$ taking into account the position information of all features of the grating.

AVA Documents
Document Sharing Hub
Full document details: PD IEC/TS 62622:2012

Note 3 to entry: The mean pitch of a grating is often also called the period length or grating constant Λ of the grating.

Note 4 to entry: For an ideal grating, the values for the mean pitch, the local pitch and the pitch for all neighboring features are identical. For real gratings, however, the values would be different, depending on the quality of the grating and the different length ranges over which the local pitch value will be evaluated. In addition, the capability of measurement methods to determine the different pitch values on non-ideal gratings is different. The measurement methods, therefore, can be classified in different groups, see 3.5.

Note 5 to entry: If the boundary length of a grating L_b (3.2.8) and the number of grating features N_f (3.2.4) are known, an approximation to the mean pitch can be determined by the equation: $p_m = L_b / (N_f - 1)$; $N_f \geq 2$. The same pitch value results if the arithmetic mean value of all pitch values over all neighboring features is calculated. In the sum $\Sigma^{Nf-1}_{i=1} (x_{i+1} - x_i) / (N_f - 1)$ for calculation of the arithmetic mean value of all pitch values of a grating all feature position values x_i cancel out except for the first and last feature. In both cases the resulting approximation of the mean pitch value is based on the positions of the first and the last feature in the grating only and thus less representative of the whole grating than the mean pitch determined by a linear regression fit [4].

3.2.6
local pitch
p_{loc} (x_c, l_r)
average pitch value determined over a defined length range l_r of a grating centered around a defined feature position x_c

EXAMPLE If a local pitch p_{loc} of a nominally 1 mm long 1D grating with 100 nm nominal pitch is evaluated around a central position at x_c = 400 µm over a length range l_r of 20 µm, the resulting local pitch should be expressed as: p_{loc} (400 µm, 20 µm) or p_{loc} (4001, 201) if expressed in number of features of the grating.

Note 1 to entry: The local pitch can also be defined over a specified number of features N_r centered around a specified feature with index N_c. In this case the notation for the local pitch is: p_{loc} (N_c, N_r).

3.2.7
nominal length of grating
L_{nom}
intended length of a grating, indicated in the specification of the grating

Note 1 to entry: The length of a grating is defined in the direction of the grating, i.e. the direction in which the number of grating features per unit length is maximal.

3.2.8
boundary length of grating
L_b
distance between the first and the last feature of a grating

Note 1 to entry: The center to center distance is the default case.

3.2.9
characteristic length of grating
L_c
length of a grating, based on the mean pitch and the number of grating features

$$L_c = p_m \cdot (N_f - 1)$$

Note 1 to entry: For an ideal grating the nominal length, the boundary length and the characteristic length values of a grating are identical. For real gratings, however, they are different.

3.3 Grating types

3.3.1
1D grating
grating in which features are repeated in only one direction within the reference plane

Documents
Document Sharing Hub
Full document details: PD IEC/TS 62622:2012

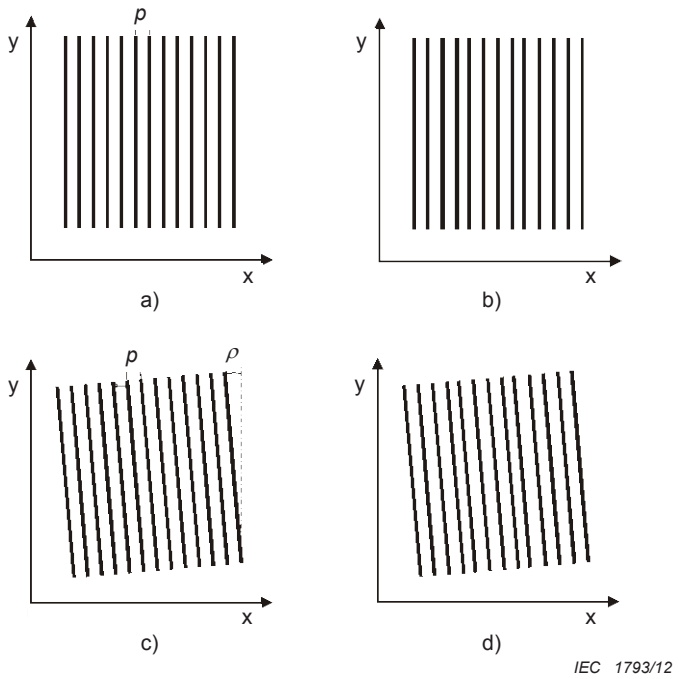

Pitch *p* is defined in the direction of the grating.

a) ideal 1D grating;

b) 1D grating with local pitch variation;

c) ideal 1D grating with misalignment by angle ρ to the instrument axes x and y;

d) 1D grating with local pitch variation and misalignment to instrument axes.

Figure 3 – Examples of 1D line gratings

EXAMPLE Figure 3 shows examples of 1D line gratings.

Note 1 to entry: 1D gratings are also denoted as one-dimensional gratings.

Note 2 to entry: According to the Note 2 to entry of 3.2.1 a line scale can be understood as a sparse 1D grating, too.

3.3.2
2D grating
grating in which features are repeated in two, non-parallel directions within the reference plane

Documents
Document Sharing Hub
Full document details: PD IEC/TS 62622:2012